

PX8000

Precision Power Scope

U S E R ' S M A N U A L

Thank you for purchasing the PX8000 Precision Power Scope (hereafter referred to as the PX8000). This User's Manual explains how to use the PX8000. To ensure correct use, please read this manual thoroughly before beginning operation.

Keep this manual in a safe place for quick reference in the event a question arises. The following manuals, including this one, are provided as manuals for the PX8000. Please read all manuals.

List of Manuals

The following four manuals, including this one, are provided as manuals for the PX8000. Read them along with this manual.

Manual Title	Manual No.	Description
PX8000 Precision Power Scope Features Guide	IM PX8000-01EN	This manual explains all the PX8000 features other than the communication interface features.
PX8000 Precision Power Scope User's Manual	IM PX8000-02EN	This manual. The manual explains how to operate the PX8000.
PX8000 Precision Power Scope Getting Started Guide	IM PX8000-03EN	Provided as a printed manual. This guide explains the handling precautions, basic operations, and specifications of the PX8000.
PX8000 Precision Power Scope Communication Interface User's Manual	IM PX8000-17EN	This manual explains the PX8000 communication interface features and how to use them.

The "EN" in the manual number is the language code.

The pdf data of all the manuals listed in the above table is in the supplied manual CD.

Contact information of Yokogawa offices worldwide is provided on the following sheet.

Document No.	Description
PIM 113-01Z2	List of worldwide contacts

Notes

- The contents of this manual are subject to change without prior notice as a result of continuing improvements to the instrument's performance and functionality. The figures given in this manual may differ from those that actually appear on your screen.
- Every effort has been made in the preparation of this manual to ensure the accuracy of its contents. However, should you have any questions or find any errors, please contact your nearest YOKOGAWA dealer.
- Copying or reproducing all or any part of the contents of this manual without the permission of YOKOGAWA is strictly prohibited.
- The TCP/IP software of this product and the documents concerning it have been developed/created by YOKOGAWA based on the BSD Networking Software, Release 1 that has been licensed from the Regents of the University of California.

Trademarks

- Microsoft, Internet Explorer, MS-DOS, Windows, Windows XP, and Windows Vista are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.
- Adobe is either registered trademark or trademark of Adobe Systems Incorporated.
- MATLAB is a registered trademark of The MathWorks, Incorporated in the United States.
- GIGAZoom ENGINE is a registered trademark of Yokogawa Electric Corporation.
- In this manual, the TM and ® symbols do not accompany their respective registered trademark or trademark names.
- Other company and product names are registered trademarks or trademarks of their respective holders.

Revisions

- January 2014 1st Edition
- January 2014 2nd Edition
- August 2014 3rd Edition

Conventions Used in This Manual

Notes

The notes and cautions in this manual are categorized using the following symbols.



Improper handling or use can lead to injury to the user or damage to the instrument. This symbol appears on the instrument to indicate that the user must refer to the user's manual for special instructions. The same symbol appears in the corresponding place in the user's manual to identify those instructions. In the user's manual, the symbol is used in conjunction with the word "WARNING" or "CAUTION."

WARNING

Calls attention to actions or conditions that could cause serious or fatal injury to the user, and precautions that can be taken to prevent such occurrences.

CAUTION

Calls attention to actions or conditions that could cause light injury to the user or cause damage to the instrument or user's data, and precautions that can be taken to prevent such occurrences.

Note

Calls attention to information that is important for the proper operation of the instrument.

Unit


k	Denotes 1000. Example: 100 kHz (frequency)
K	Denotes 1024. Example: 720 KB (file size)

Key and Jog Shuttle Operations

Key Operations

How to Use Setup Menus That Appear When Keys Are Pressed

The operation after you press a key varies depending on the key that you press.

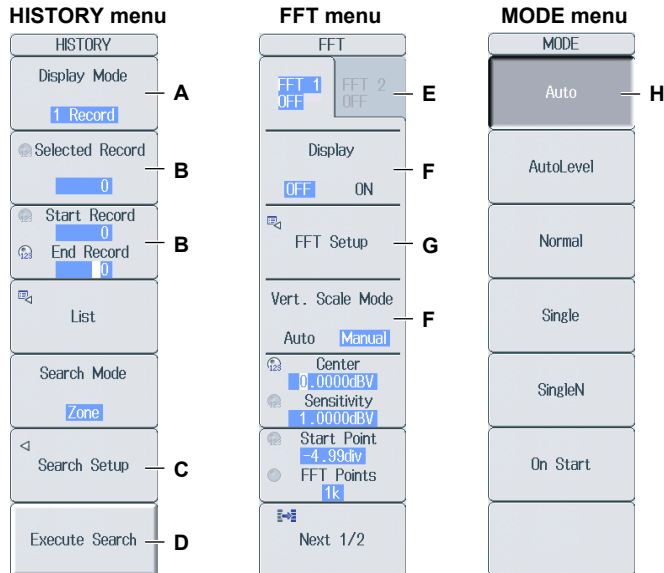

- A: Press the soft key to display a selection menu.
Press the soft key that corresponds to the appropriate setting.
- B: Press the soft key to use the jog shuttle to configure this setting. Use the jog shuttle or the arrow keys to set the value or select an item.
For a numeric setting, you can press NUM LOCK to use the ELEM 1 to P 4 keys to enter numbers.
- C: A related setup menu appears when you press the soft key.
- D: Press the soft key to execute the specified feature.
- E: Selects which item to configure when configuring a feature that consists of two items that operate with different settings, such as the FFT1 and FFT2 features.
- F: The selected setting switches each time you press the soft key.
- G: A dialog box or the keyboard appears when you press the soft key.
Use the jog shuttle, SET key, and arrow keys to configure the settings in the dialog box or operate the keyboard.
- H: Press the soft key to apply the value assigned to the key.

How to Display the Setup Menus That Are Written in Purple below the Keys

In the explanations in this manual, "SHIFT+key name (written in purple)" is used to indicate the following operation.

1. Press **SHIFT**. The SHIFT key illuminates to indicate that the keys are shifted.
Now you can select the setup menus written in purple in the manual.
2. Press the key that you want to display the setup menu of.

ESC Key Operation

If you press **ESC** when a setup menu or available options are displayed, the screen returns to the menu level above the current one. If you press **ESC** when the highest level menu is displayed, the setup menu disappears.

RESET Key Operation

If you press **RESET** when you are using the jog shuttle to set a value or select an item, the setting is reset to its default value (depending on the operating state of the PX8000, the setting may not be reset).

SET Key Operations

The operation varies as indicated below depending on what you are setting.

- For a soft key menu that has two values that you use the jog shuttle to adjust
Press **SET** to switch the value that the jog shuttle adjusts.
- For a menu that has the jog shuttle + SET mark (⊖+⊕) displayed on it
Press **SET** to confirm the selected item.

Arrow Key Operations


The operation varies as indicated below depending on what you are setting.

- When setting a value
 - Up and down **arrow** keys: Increases and decreases the value
 - Left and right **arrow** keys: Changes which digit to set
- When selecting the item to set
 - You can use the up, down, left, and right arrow keys.


How to Enter Values in Setup Dialog Boxes

1. Use the keys to display the appropriate setup dialog box.
2. Use the **jog shuttle** or the **arrow** keys to move the cursor to the setting that you want to set.
3. Press **SET**. The operation varies as indicated below depending on what you are setting.
 - A selection menu appears.
 - A check box is selected or cleared.
 - An item is selected.
 - A table of settings is selected.

Displaying a Selection Menu and Selecting an Item

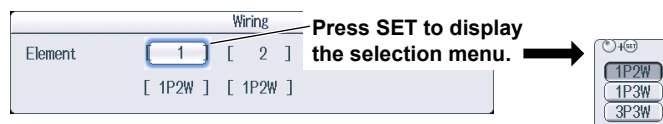

After selecting an item with the jog shuttle, press SET to confirm it.

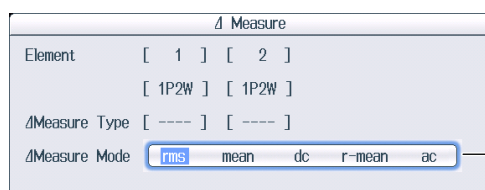

Setting Items in a Table

Judgement Setup

#	Mode	Trace	Item	Upper	Lower
1	IN	U1	Peak to Peak	0.0000	0.0000
2	X	U1	Peak to Peak	0.0000	0.0000
3	X	U1	Peak to Peak	0.0000	0.0000
4	X	U1	Peak to Peak	0.0000	0.0000
5	X	U1	Peak to Peak	0.0000	0.0000
6	X	U1	Peak to Peak	0.0000	0.0000
7	X	U1	Peak to Peak	0.0000	0.0000
8	X	U1	Peak to Peak	0.0000	0.0000
9	X	U1	Peak to Peak	0.0000	0.0000
10	X	U1	Peak to Peak	0.0000	0.0000
11	X	U1	Peak to Peak	0.0000	0.0000
12	X	U1	Peak to Peak	0.0000	0.0000
13	X	U1	Peak to Peak	0.0000	0.0000
14	X	U1	Peak to Peak	0.0000	0.0000
15	X	U1	Peak to Peak	0.0000	0.0000
16	X	U1	Peak to Peak	0.0000	0.0000

Logic: **AND** OR

ActCondition: Always **Fail** Success

After moving the cursor to the table, press SET to select the setting in the table that you want to change.
To exit from the list, press ESC.

#	Mode	Trace	Item
1	IN	U1	Peak to Peak
2	X	U1	Peak to Peak
3	X	U1	Peak to Peak

Press SET to select the item that you want to set.

How to Clear Setup Dialog Boxes

Press **ESC** to clear the setup dialog box from the screen.

Entering Values and Strings

Entering Values

Using Dedicated Knobs

You can use the following dedicated knobs to enter values directly.


- **◆**POSITION knob (vertical POSITION knob)
- RANGE knob
- TIME/DIV knob
- MAG knob (magnification knob)
- **◀**POSITION**▶** knob (zoom POSITION knob)

Using the Jog Shuttle

Select the appropriate item using the soft keys, and change the value using the jog shuttle and the SET key or using the arrow keys. This manual sometimes describes this operation simply as “using the jog shuttle.”

Using the Keypad

Press **NUM LOCK** to illuminate the NUM LOCK key, and use the ELEM1 to P4 keys to enter a value. After you enter the value, press **ENTER** to confirm it.

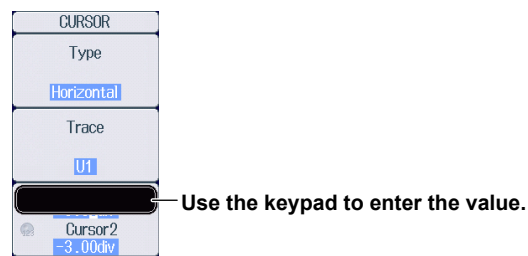


Note


Some items that you can set using the jog shuttle are reset to their default values when you press the RESET key.

Entering Character Strings


Use the keyboard that appears on the screen to enter character strings such as file names and comments. Use the jog shuttle, SET key, and arrow keys to operate the keyboard and enter a character string.

How to Operate the Keyboard

1. After bringing up the keyboard, use the **jog shuttle** to move the cursor to the character that you want to enter. You can also move the cursor using the up, down, left, and right **arrow** keys.
2. Press SET to enter the character.
 - If a character string has already been entered, use the **arrow** soft keys (< and >) to move the cursor to the position you want to insert characters into.
 - To switch between uppercase and lowercase letters, press the **Caps** soft key or move the cursor to **CAPS** on the keyboard, and then press **SET**.
 - To delete the previous character, press the **Back Space** soft key.
 - To delete all the characters, press the **All Clear** soft key.
3. Repeat steps 1 and 2 to enter all of the characters in the string.
 Select  on the keyboard or press the **History** soft key to display a list of character strings that you have entered previously. Use the jog shuttle to select a character string, and press **SET** to enter the selected character string.
4. Press the **Enter** soft key, or move the cursor to ENTER on the keyboard, and press **SET**.
 The character string is confirmed, and the keyboard disappears.

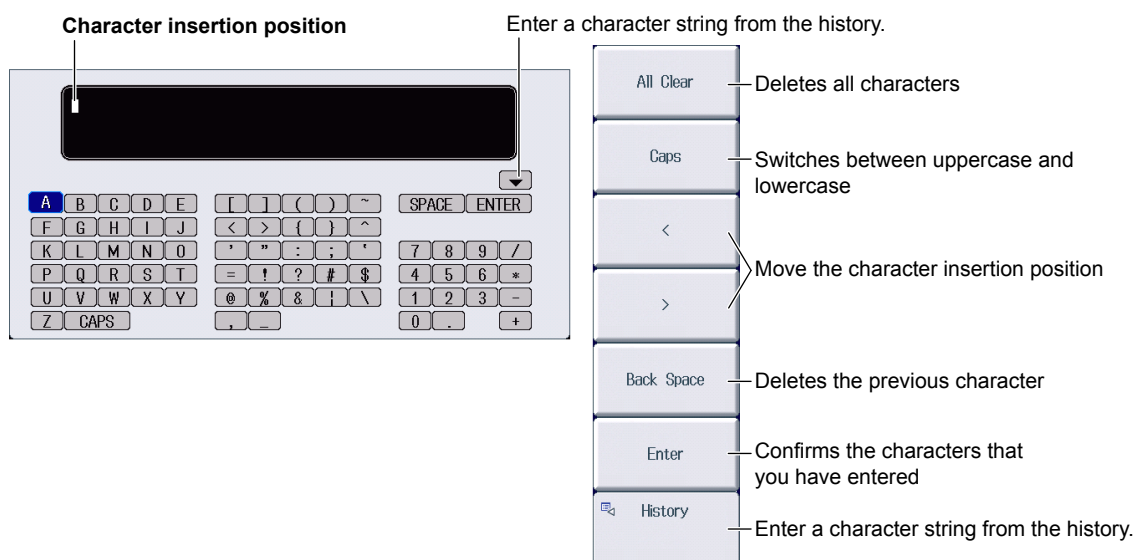

History (a list of character strings that you have entered previously)

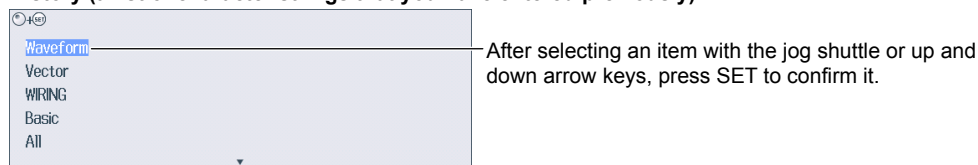

Note

- @ cannot be entered consecutively.
- File names are not case-sensitive. Comments are case-sensitive. The following file names cannot be used due to MS-DOS limitations:
 AUX, CON, PRN, NUL, CLOCK, COM1 to COM9, and LPT1 to LPT9
 For details on file name limitations, see the Features Guide, IM PX8000-01EN.
- When a character string is confirmed, it is stored in a list of previously entered strings. Up to 50 character strings are stored. The new character string appears at the top of the list of previously entered strings.

Contents

Conventions Used in This Manual	iii
Key and Jog Shuttle Operations	iv
Entering Values and Strings.....	vii

Chapter 1 Fundamental Measurement Conditions

1.1 Configuring Wiring System Settings	1-1
1.2 Configuring Power Measurement Element Settings	1-3
1.3 Setting the Motor Mode	1-4

Chapter 2 Vertical and Horizontal Control

2.1 Configuring Voltage Measurements	2-1
2.2 Configuring Current Measurements	2-4
2.3 Configuring Power Measurements	2-8
⚠ 2.4 Configuring Sensor Input Voltage Measurements	2-10
2.5 Configuring Rotating Speed Measurements	2-17
2.6 Configuring Torque Measurements	2-23
2.7 Displaying the Menu for Configuring All Channels	2-29
2.8 Configuring the Horizontal Axis (Time axis).....	2-31

Chapter 3 Triggering

3.1 Setting the Trigger Mode	3-1
3.2 Setting the Trigger Position and Trigger Delay	3-2
3.3 Setting the Trigger Hold Off	3-3

Simple trigger

3.4 Triggering on an Edge Trigger (Simple)	3-4
3.5 Triggering on a Timer Trigger (Simple).....	3-5
3.6 Triggering on an External Trigger (Simple).....	3-6
3.7 Triggering on a Power Line Signal (Simple).....	3-7

Enhanced trigger

3.8 Triggering on an A -> B(N) Trigger (Enhanced).....	3-8
3.9 Triggering on an A Delay B Trigger (Enhanced)	3-9
3.10 Triggering on an Edge On A Trigger (Enhanced)	3-10
3.11 Triggering on an OR or AND Trigger (Enhanced).....	3-11
3.12 Triggering on a Period Trigger (Enhanced)	3-13
3.13 Triggering on a Pulse Width Trigger (Enhanced)	3-15
3.14 Triggering on a Wave Window Trigger (Enhanced).....	3-17

Manual trigger

3.15 Triggering the PX8000 Manually (Manual Trigger).....	3-18
---	------

Chapter 4 Waveform Acquisition

4.1 Setting Conditions for Waveform Acquisition.....	4-1
4.2 Starting and Stopping Waveform Acquisition	4-3

Chapter 5 Display Mode

5.1 Selecting the Display Mode	5-1
--------------------------------------	-----

Chapter 6 Numeric Data Display

6.1	Switching the Displayed Page.....	6-1
6.2	Changing the Displayed Items on the 4-, 8-, and 16-Value Displays	6-3
6.3	Changing the Displayed Items on the Matrix Display.....	6-5
6.4	Changing the All Items Display.....	6-7
6.5	Changing the Harmonics List Display (Option)	6-8
6.6	Setting the Custom Display	6-10

Chapter 7 Numeric Computation

7.1	Turning Numeric Measurement On and Off	7-1
7.2	Setting the Calculation Period	7-2
7.3	Setting Numeric Data Averaging	7-3
7.4	Setting User-Defined Functions	7-4
7.5	Setting Apparent Power, Reactive Power, and Corrected Power Equations.....	7-6
7.6	Setting the Phase Difference Display Format.....	7-8
7.7	Setting Harmonic Measurement Conditions.....	7-9

Chapter 8 Waveform Display

8.1	Setting the Waveform Display	8-1
8.2	Using the Snapshot and Clear Trace Features	8-3

Chapter 9 Bar Graph Display (Option)

9.1	Configuring the Bar Graph Display.....	9-1
-----	--	-----

Chapter 10 Vector Display (Option)

10.1	Configuring the Vector Display	10-1
------	--------------------------------------	------

Chapter 11 X-Y Display

11.1	Displaying X-Y Waveforms.....	11-1
------	-------------------------------	------

Chapter 12 Zooming Waveforms

12.1	Zooming in on or out of Waveforms	12-1
------	---	------

Chapter 13 Cursor Measurement

13.1	Measuring with Horizontal Cursors	13-1
13.2	Measuring with Vertical Cursors.....	13-2
13.3	Measuring with Marker Cursors (Marker).....	13-3
13.4	Measuring with Angle Cursors (Degree)	13-5
13.5	Measuring with Horizontal and Vertical Cursors (H & V).....	13-6
13.6	Measuring with Peak Cursors (Peak).....	13-7

Chapter 14 Automated Measurement of Waveform Parameters

14.1	Automatically Measuring Waveform Parameters	14-1
14.2	Performing Normal Statistical Processing	14-4
14.3	Performing Cyclic Statistical Processing	14-5

Chapter 15 Waveform Computation

15.1	Performing Addition, Subtraction, Multiplication, and Division	15-1
15.2	Performing Binary Conversion	15-2
15.3	Shifting the Phase	15-3
15.4	Displaying the Power Spectrum	15-4
15.5	Performing User-Defined Computations	15-5

Chapter 16 FFT

16.1	Displaying FFT Waveforms	16-1
------	--------------------------------	------

Chapter 17 GO/NO-GO Determination

17.1	Performing GO/NO-GO Determination with Waveform Zones	17-1
17.2	Performing GO/NO-GO Determination with Waveform Parameters	17-4

Chapter 18 Action

18.1	Setting Actions	18-1
------	-----------------------	------


Chapter 19 Searching Waveforms

19.1	Searching for Edges	19-1
19.2	Searching for a Specific Time	19-3


Chapter 20 Displaying and Searching History Waveforms

20.1	Displaying Waveform History Waveforms	20-1
20.2	Searching History Waveforms	20-3

Chapter 21 Printing and Saving Screen Captures

 21.1	Loading Roll Paper Into the Built-In Printer (Optional)	21-1
21.2	Printing on the Built-in Printer (Option)	21-3
21.3	Saving Screen Captures to Files	21-4

Chapter 22 Saving and Loading Data

 22.1	Connecting Storage Media	22-1
22.2	Formatting Storage Media	22-4
22.3	Saving Waveform Data	22-6
22.4	Saving Numeric Data	22-11
22.5	Saving Setup Data	22-14
22.6	Saving Other Types of Data	22-15
22.7	Loading Waveform Data	22-19
22.8	Loading Setup Data	22-20
22.9	Loading Other Types of Data	22-21
22.10	Performing File Operations	22-22

Chapter 23 Ethernet Communication

23.1	Connecting the PX8000 to a Network	23-1
23.2	Configuring TCP/IP Settings	23-3
23.3	Accessing the PX8000 from a PC (FTP Server)	23-4
23.4	Connecting to a Network Drive	23-5
23.5	Using SNTP to Set the Date and Time	23-6

Chapter 24 Other Operations

24.1	Calibrating the PX8000	24-1
24.2	Using the NULL Feature	24-2
24.3	Setting Time Synchronization (Option)	24-3
24.4	Changing the Message, Menu, and USB Keyboard Languages	24-4
24.5	Adjusting the Backlight	24-5
24.6	Initializing the Settings	24-6
24.7	Configuring the Environment Settings	24-7
24.8	Storing and Recalling Setup Data	24-9
24.9	Locking the Keys	24-10

Chapter 25 Messages and Self-Test

25.1	Messages and Corrective Actions	25-1
25.2	Carrying Out Self-Tests (Selftest)	25-8
25.3	Viewing System Information (Overview).....	25-11

Index

1.1 Configuring Wiring System Settings


This section explains the following wiring system settings.

- Wiring system
- Efficiency equation
- Turning independent element configuration on and off
- Delta computation
- Display format of external current sensor range
- Deskewing (correcting the transfer time difference between input signals)

► **Features Guide: “Wiring System Settings (WIRING)”**

WIRING Menu

Press **WIRING** to display the following menu.

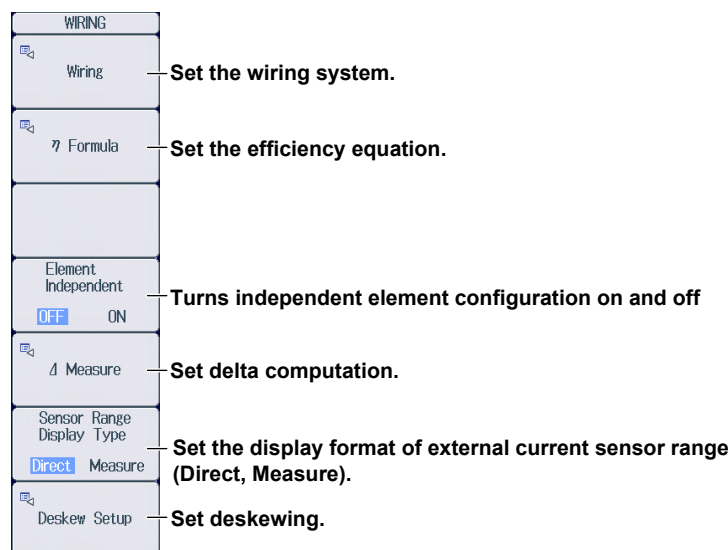


Setting the Wiring System

Press the **Wiring** soft key to display the following screen.

Set the wiring system (1P2W, 1P3W, 3P3W, 3P4W, 3P3W(3V3A)).

When you select an element, the wiring systems that you can select are displayed. Select the wiring system from those displayed.

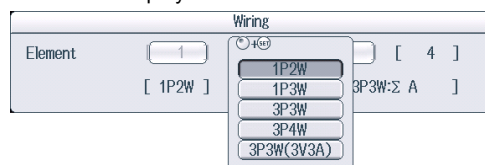

Wiring System Combination

- If you select 1P3W, 3P3W, 3P4W, or 3P3W(3V3A) for the wiring system, the wiring unit is set with the two or three elements adjacent to the selected element whose element numbers are larger than the selected element.
- On models that have four elements installed, up to two wiring units (ΣA and ΣB) are automatically set. The wiring unit symbols ΣA and ΣB are attached to the element numbers in order, starting with the smallest number.

Note

- Because the wiring system with the largest element number is automatically determined according to the settings of the wiring system with the smallest element number, the element with the largest element number cannot be selected.
- You cannot set the wiring units for larger element numbers before the wiring units for smaller element numbers.

Setting the Efficiency Equation (η Formula)

Press the η Formula soft key to display the following screen.

Element

[1] [2] [3] [4]

[3P3W-Σ A] [1P3W-Σ B]

PΣB

PΣA

PΣA

PΣB

OFF

OFF

η1 =

η2 =

η3 =

η4 =

100[%]

100[%]

100[%]

100[%]

Udef1 =

Udef2 =

P1

P1

None

None

None

None

None

None

Installed elements

The set wiring systems

Set the denominator and numerator of the efficiency equation to the active power and motor power measurement functions.
(P1-P4¹, PΣA-PΣB², Pm2-Pm4³, Udef1, Udef2)
You can set up to four equations: η1 to η4.

Define Udef1 and Udef2
(P1-P4¹, PΣA-PΣB², Pm2-Pm4³).

To add active powers and motor output and use them in efficiency equations, use Udef1 and Udef2.

- 1 P1 to P4 can be set within the range of the installed elements.
- 2 PΣA to PΣB can be set within the range of the wiring unit that is automatically determined by the installed elements.
- 3 Pm2, Pm3, and Pm4 can be set when AUX modules are installed in slots 3, 5, and 7, respectively.

Setting Delta Computation (Δ Measure)

Press the Δ Measure soft key to display the following screen.

Element

[1] [2] [3] [4]

[3P3W-Σ A] [1P3W-Σ B]

ΔMeasure Type

3P3W>3V3A

Difference

ΔMeasure Mode

rms

mean

dc

r-mean

ac

Installed elements

The set wiring systems

Set the delta computation type.
The available options vary depending on the set wiring systems.

Wiring System	Delta Computation Type
1P3W	Difference, 3P3W>3V3A
3P3W	Difference, 3P3W>3V3A
3P4W	Star>Delta
3P3W(3V3A)	Delta>Star

Set the delta computation mode (rms, mean, dc, r-mean, ac).

Setting Deskewing (Deskew Setup)

Press the Deskew Setup soft key to display the following screen.

Deskew Setup

All

U1/I1

U2/I2

U3/I3

U4/I4

Diff Time U

0.000 ns

0.000 ns

0.000 ns

0.000 ns

Diff Time I

0.000 ns

0.000 ns

0.000 ns

0.000 ns

Diff Time Sen

0.000 ns

0.000 ns

0.000 ns

0.000 ns

Voltage (U) or current (I) of the installed elements

Manual deskewing

- Set the correction value for voltage signals.
- Set the correction value for current signals.
- Set the correction value for external current sensor signals.

To set or execute on all channels, set or execute the items in the All row.

1-2

IM PX8000-02EN

1.2 Configuring Power Measurement Element Settings

This section explains the following element settings.

- Line filter
- Frequency filter
- Turning the scaling feature on and off
- VT ratio
- CT ratio
- Power coefficient
- Synchronization source

► [Features Guide: “Power Measurement Element Settings \(ELEM1 to 4\)”](#)

Check that a voltage module and current module are installed in appropriate slots.

ELEM Menu

Of the **ELEM1** to **ELEM4** keys, press the key corresponding to the element in which the voltage and current modules are installed. The following menu appears.

ELEM1	
Line Filter OFF	Set the line filter (OFF, 500Hz, 2kHz, 20kHz, 1MHz).
Freq Filter OFF	Set the frequency filter (OFF, 100Hz, 500Hz, 2kHz, 20kHz).
Scaling OFF ON	Turns the scaling feature on and off*
VT Scaling 1.0000	Set the VT ratio.
CT Scaling 1.0000	Set the CT ratio.
SF Scaling 1.0000	Set the power coefficient.
Sync Source I1	Set the synchronization source (U1-U4, I1-I4, External, None).

* When you are trying to read the current of the circuit under measurement directly by multiplying the external current sensor output by the conversion ratio, if the scaling feature is set to ON, the CT ratio will end up being multiplied on top of the result. To avoid the influence of the CT ratio, set the CT ratio to 1.0000.

1.3 Setting the Motor Mode

This section explains the following motor mode settings.

- Turning motor mode on and off
- Function name
- Scaling
- Unit
- Synchronization source

► **Features Guide: “Turning Motor Mode On and Off (Motor Mode)”**
“Function Name (Name)”
“Scaling (Scaling)”
“Unit (Unit)”
“Synchronization Source (Sync Source), AUX Module”

Check that an AUX module is installed in slot 3, 5, or 7.

Pm Menu

Of the **ELEM 2 to ELEM 4** keys, press the key corresponding to the slot in which the AUX module is installed. The following menu appears.

When motor mode is off

Pm3	
Motor Mode	Set Motor Mode to OFF.
OFF ON	
Name	
None	
Scaling	
1.0000	
Unit	
W	
Sync Source	Set the synchronization source (U1-U4, I1-I4, External, None).
None	

When motor mode is on

Pm3	
Motor Mode	Set Motor Mode to ON.
OFF ON	
Name	Set the function name.
Pm3	
Scaling	Set the scaling.
1.0000	
Unit	Set the unit.
W	
Sync Source	Set the synchronization source (U1-U4, I1-I4, External, None).
None	

2.1 Configuring Voltage Measurements

This section explains the following settings for the vertical axis of voltage measurements.

- Waveform display on and off
- Display labels
- Zoom method
 - DIV: Magnification for zooming waveforms, offset
 - SPAN: Upper and lower display limits for zooming waveforms
- Auto range on and off
- Voltage measurement range (vertical scale)
- Voltage waveform vertical position

► [Features Guide: “Voltage Measurement \(U\)”](#)

Check that a voltage module and current module are installed in appropriate slots.

U Menu

Of the **U1** to **U4** keys, press the key corresponding to the element in which the module is installed. The following menu appears.

When the zoom method is set to DIV

U1 (CH1)

Display

OFF ON

Label

U1

Vertical Scale

DIV SPAN

Vertical Zoom

X 1

Offset

0.0V

Auto Range

OFF ON

Turns the waveform display on and off

Set the display label.

Set the zoom method to DIV.

Set the zoom magnification.

Set the offset.

Turns the auto range on and off

When the zoom method is set to SPAN

U1 (CH1)

Display

OFF ON

Label

U1

Vertical Scale

DIV SPAN

Upper

250.0V

Lower

-250.0V

Auto Range

OFF ON

Turns the waveform display on and off

Set the display label.

Set the zoom method to SPAN.

Set the upper and lower limits of the display range.

Turns the auto range on and off

Note The U key whose display setting is ON illuminates. If the U key is not illuminated, you can press it to turn on the waveform display and the key. If the U key is illuminated, you can press it to turn off the waveform display and the key.

Setting the Voltage Measurement Range (Vertical Scale, RANGE Knob)

This section explains how to set a fixed range.

(If Auto Range in the U menu is set to ON, the measurement range changes depending on the amplitude of the input signal.)


Turn the **RANGE** knob to set the voltage measurement range.

- Select from 1.5V, 3V, 6V, 10V, 15V, 30V, 60V, 100V, 150V, 300V, 600V, and 1000V.
- Auto Range in the U menu is set to OFF.
- If you turn the RANGE knob when waveform acquisition is stopped, two values are shown on the measurement range screen. The upper value is the measurement range for the displayed waveforms. The lower value is the measurement range that you have specified. The new range will be applied the next time waveform acquisition is started.
- If you do not operate the RANGE knob for approximately 3 seconds, the measurement range that you are setting with the knob will disappear from the screen.

Top row: Measurement range for the displayed waveforms

Bottom row: Measurement range that you have specified

When the displayed waveform's measurement range and the measurement range that you have set are the same, only the bottom row is displayed.



Use the RANGE knob to display the measurement range that is currently being set.

Range status

Indicates the wiring units.

Display example

When the wiring system is 1P2W



Because the wiring unit is separate for each element, set the measurement range of each element.

When the wiring system is 1P3W or 3P3W



Element 1 (CH1, CH2) and element 2 (CH3, CH4) are grouped into a single wiring unit. Changing the measurement range of one element will change that of the other element to the same value.*

* If independent element configuration (see section 1.1) to ON, you need to set the measurement range for each element.

Setting the Voltage Waveform Vertical Position

When the Zoom Method is Set to DIV (Vertical POSITION Knob)


Turn the **vertical POSITION** knob to set the waveform vertical position.

- Set in the range of -5.00 div to 5.00 div.
- If you do not operate the vertical POSITION knob for approximately 3 seconds, the vertical position that you are setting with the knob will disappear from the screen.



Use the vertical **POSITION** knob to display the vertical position that is currently being set.


- You can set the vertical position to 0 div by pressing the knob.



This indicates that you can press the vertical **POSITION** knob to set the vertical position to 0 div.

When the Zoom Method is Set to SPAN (Upper and Lower Limits)

Using the **Upper/Lower** soft key and the **jog shuttle**, set the voltage at the top edge of the waveform screen (upper limit) and the voltage at the bottom edge of the screen (lower limit) to set the waveform vertical position.

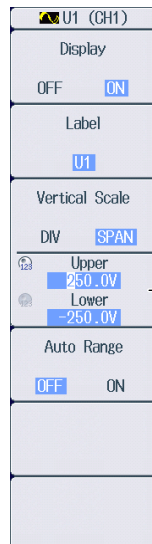

Set the upper and lower limits of the display range.

2.2 Configuring Current Measurements

This section explains the following settings for the vertical axis of current measurements.

- Waveform display on and off
- Display labels
- Zoom method
 - DIV: Magnification for zooming waveforms, offset
 - SPAN: Upper and lower display limits for zooming waveforms
- Auto range on and off
- Current measurement range (vertical scale)
 - Direct input, external current sensor (conversion ratio, input coupling)
- Current waveform vertical position

► [Features Guide: “Current Measurement \(I\)”](#)

Check that a voltage module and current module are installed in appropriate slots.

I Menu

Of the **I1** to **I4** keys, press the key corresponding to the element in which the module is installed. The following menu appears.

When the zoom method is set to DIV

Turns the waveform display on and off

Set the display label.

Set the zoom method to DIV.

Set the zoom magnification.

Set the offset.

Turns the auto range on and off

Turns the external current sensor on and off*

Set the external current sensor conversion ratio.*
Set this when the external current sensor (Ext Sensor) is set to ON.

When the zoom method is set to SPAN

Turns the waveform display on and off

Set the display label.

Set the zoom method to SPAN.

Set the upper and lower limits of the display range.

Turns the auto range on and off

Turns the external current sensor on and off*

Set the external current sensor conversion ratio.*
Set this when the external current sensor (Ext Sensor) is set to ON.

- In the case of a 760813 (current module), Ext Sensor and Sensor Ratio do not appear.

Note

The **I** key whose display setting is ON illuminates. If the **I** key is not illuminated, you can press it to turn on the waveform display and the key. If the **I** key is illuminated, you can press it to turn off the waveform display and the key.

Setting the Current Measurement Range (Vertical Scale, RANGE Knob)

This section explains how to set a fixed range.

(If Auto Range in the I menu is set to ON, the measurement range changes depending on the amplitude of the input signal.)

Direct Input Measurement Range Settings (When Ext Sensor is set to OFF)


Turn the **RANGE** knob to set the current measurement range.

- Select from 10mA, 20mA, 50mA, 100mA, 200mA, 500mA, 1A, 2A, and 5A.
- Auto Range in the I menu is set to OFF.
- If you turn the RANGE knob when waveform acquisition is stopped, two values are shown on the measurement range screen. The upper value is the measurement range for the displayed waveforms. The lower value is the measurement range that you have specified. The new range will be applied the next time waveform acquisition is started.
- If you do not operate the RANGE knob for approximately 3 seconds, the measurement range that you are setting with the knob will disappear from the screen.

Top row: Measurement range for the displayed waveforms

Bottom row: Measurement range that you have specified

When the displayed waveform's measurement range and the measurement range that you have set are the same, only the bottom row is displayed.



Use the RANGE knob to display the measurement range that is currently being set.

Range status

Indicates the wiring units.

Display example

When the wiring system is 1P2W



Because the wiring unit is separate for each element, set the measurement range of each element.

When the wiring system is 1P3W or 3P3W



Element 1 (CH1, CH2) and element 2 (CH3, CH4) are grouped into a single wiring unit. Changing the measurement range of one element will change that of the other element to the same value.*

* If independent element configuration (see section 1.1) to ON, you need to set the measurement range for each element.

External Current Sensor Input Measurement Range Settings (When Ext Sensor is set to ON)

When the External Current Sensor Range Display Format (see section 1.1) Is Direct


Turn the **RANGE** knob to set the current measurement range.

- Select from 50mV, 100mV, 200mV, 500mV, 1V, 2V, 5V, and 10V.
- Auto Range in the I menu is set to OFF.
- If you turn the RANGE knob when waveform acquisition is stopped, two values are shown on the measurement range screen. The upper value is the measurement range for the displayed waveforms. The lower value is the measurement range that you have specified. The new range will be applied the next time waveform acquisition is started.
- If you do not operate the RANGE knob for approximately 3 seconds, the measurement range that you are setting with the knob will disappear from the screen.

Top row: Measurement range for the displayed waveforms

Bottom row: Measurement range that you have specified

When the displayed waveform's measurement range and the measurement range that you have set are the same, only the bottom row is displayed.



Range status
See page 2-5.

Use the RANGE knob to display the measurement range that is currently being set.

When the External Current Sensor Range Display Format (see section 1.1) Is Measure


Turn the **RANGE** knob to set the current measurement range.

- Select from 50mV, 100mV, 200mV, 500mV, 1V, 2V, 5V, and 10V.
- Auto Range in the I menu is set to OFF.
- If you turn the RANGE knob when waveform acquisition is stopped, two values are shown on the measurement range screen. The upper value is the measurement range for the displayed waveforms. The lower value is the measurement range that you have specified. The new range will be applied the next time waveform acquisition is started.
- If you do not operate the RANGE knob for approximately 3 seconds, the measurement range that you are setting with the knob will disappear from the screen.

Top row: Measurement range for the displayed waveforms

Bottom row: Measurement range that you have specified

- The measurement range is set to the value that results when the measurement range set with the RANGE knob is divided by the external current sensor conversion ratio (see page 2-4).
- When the displayed waveform's measurement range and the measurement range that you have set are the same, only the bottom row is displayed.



Range status
See page 2-5.


Use the RANGE knob to display the measurement range that is currently being set.

Setting the Current Waveform Vertical Position

When the Zoom Method is Set to DIV (Vertical POSITION Knob)


Turn the **vertical POSITION** knob to set the waveform vertical position.

- Set in the range of -5.00 div to 5.00 div.
- If you do not operate the vertical POSITION knob for approximately 3 seconds, the vertical position that you are setting with the knob will disappear from the screen.

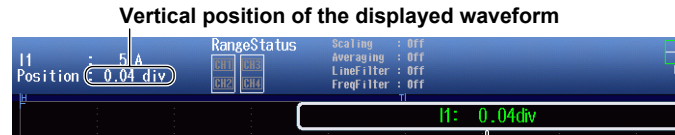

Use the vertical **POSITION** knob to display the vertical position that is currently being set.


- You can set the vertical position to 0 div by pressing the knob.



This indicates that you can press the vertical **POSITION** knob to set the vertical position to 0 div.

When the Zoom Method is Set to SPAN (Upper and Lower Limits)

Using the **Upper/Lower** soft key and the **jog shuttle**, set the current at the top edge of the waveform screen (upper limit) and the current at the bottom edge of the screen (lower limit) to set the waveform vertical position.

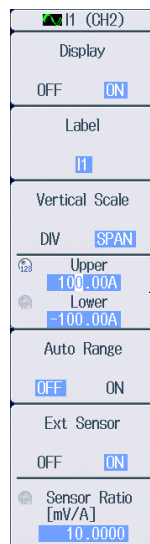

Set the upper and lower limits of the display range.

2.3 Configuring Power Measurements

This section explains the following settings for the vertical axis of power measurements.

- Waveform display on and off
- Display labels
- Zoom method
 - DIV: Magnification for zooming waveforms, offset
 - SPAN: Upper and lower display limits for zooming waveforms
- Power waveform vertical position

► [Features Guide: “Power Measurement \(P\)”](#)

Check that a voltage module and current module are installed in appropriate slots.

POWER Menu

Of the **P1** to **P4** keys, press the key corresponding to the element in which the module is installed. The following menu appears.

When the zoom method is set to DIV

POWER1

Display

OFF ON

Label

P1

Vertical Scale

DIV SPAN

Vertical Zoom

x 2

Offset

0W

Turns the waveform display on and off

Set the display label.

Set the zoom method to DIV.

Set the zoom magnification.

Set the offset.

When the zoom method is set to SPAN

POWER1

Display

OFF ON

Label

P1

Vertical Scale

DIV SPAN

Upper

1000.0W

Lower

-1000.0W

Turns the waveform display on and off

Set the display label.

Set the zoom method to SPAN.

Set the upper and lower limits of the display range.

Note


The P key whose display setting is ON illuminates. If the P key is not illuminated, you can press it to turn on the waveform display and the key. If the P key is illuminated, you can press it to turn off the waveform display and the key.

Setting the Power Waveform Vertical Position

When the Zoom Method is Set to DIV (Vertical POSITION Knob)


Turn the **vertical POSITION** knob to set the waveform vertical position.

- Set in the range of -5.00 div to 5.00 div.
- If you do not operate the vertical POSITION knob for approximately 3 seconds, the vertical position that you are setting with the knob will disappear from the screen.

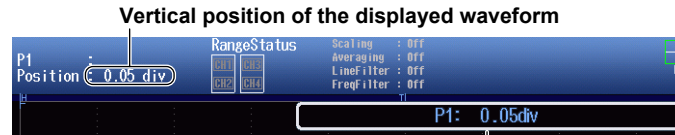

Use the vertical **POSITION** knob to display the vertical position that is currently being set.


- You can set the vertical position to 0 div by pressing the knob.



This indicates that you can press the vertical **POSITION** knob to set the vertical position to 0 div.

When the Zoom Method is Set to SPAN (Upper and Lower Limits)

Using the **Upper/Lower** soft key and the **jog shuttle**, set the power at the top edge of the waveform screen (upper limit) and the power at the bottom edge of the screen (lower limit) to set the waveform vertical position.

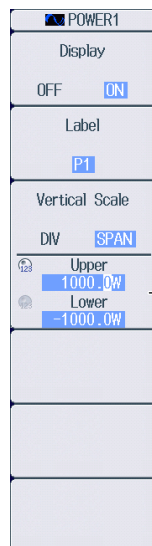

Set the upper and lower limits of the display range.

2.4 Configuring Sensor Input Voltage Measurements

This section explains the following settings for the vertical axis of sensor input voltage measurements.

- Waveform display on and off
- Display labels
- Zoom method
 - DIV: Magnification for zooming waveforms, offset
 - SPAN: Upper and lower display limits for zooming waveforms
- Auto range on and off
- AUX settings
 - Input signal type, linear scaling, display format
- Input coupling
- Probe attenuation
- Bandwidth limit
- Upper and lower pulse reference levels
- Sensor input voltage measurement range
- Sensor input voltage waveform vertical position

► [Features Guide: “Sensor Input Voltage Measurement \(AUX\)”](#)

Check that an AUX module is installed in slot 3, 5, or 7.

Pm Menu

Of the **ELEM 2 to ELEM 4** keys, press the key corresponding to the slot in which the AUX module is installed. On the menu that appears, set Motor Mode to OFF.

The screenshot shows a vertical menu titled "Pm3". The menu items are: "Motor Mode" with "OFF" and "ON" options; "Name" with a blue button; "Scaling" with a blue button; "Unit" with a blue button; and "Sync Source" with a "None" button. Annotations point to the "OFF" option under "Motor Mode" and the "None" option under "Sync Source".

Set Motor Mode to OFF.

Set the synchronization source. ► section 1.3

AUX Menu

- Press **U2(CH3)**, **I2(CH4)**, **U3(CH5)**, **I3(CH6)**, **U4(CH7)**, or **I4(CH8)** to select a channel on an installed AUX module. The following menu appears.

When the zoom method is set to **DIV**

Display	Turns the waveform display on and off
Label	Set the display label.
Vertical Scale	Set the zoom method to DIV.
Vertical Zoom	Set the zoom magnification.
Offset	Set the offset.
Auto Range	Turns the auto range on and off*
Aux Settings (Analog/Pulse)	AUX settings
Next 1/2	Displays the second page of the menu

When the zoom method is set to **SPAN**

Display	Turns the waveform display on and off
Label	Set the display label.
Vertical Scale	Set the zoom method to SPAN.
Upper/Lower	Set the upper and lower limits of the display range.
Auto Range	Turns the auto range on and off*
Aux Settings (Analog/Pulse)	AUX settings
Next 1/2	Displays the second page of the menu

* You can turn auto range on and off when the AUX input signal type is set to Analog. If the type is set to Pulse, auto range is fixed to OFF.

Note

The U or I key whose display setting is ON illuminates. If the U or I key is not illuminated, you can press it to turn on the waveform display and the key. If the U or I key is illuminated, you can press it to turn off the waveform display and the key.

- Press the **Next 1/2** soft key to display the 2/2 menu.

When the AUX input signal type is **Analog**

Coupling	Set the input coupling (AC, DC, GND).
Probe	Set the probe attenuation (1:1, 10:1, 100:1, 1000:1).
Bandwidth	Set the bandwidth limit (10kHz, 20kHz, 40kHz, 80kHz, 160kHz, 320kHz, 640kHz, 1.28MHz, 2MHz, Full).
Pulse Level High	
Pulse Level Low	
Next 2/2	Displays the first page of the menu

When the AUX input signal type is **Pulse**

Coupling	
Probe	
Bandwidth	Set the bandwidth limit (10kHz, 20kHz, 40kHz, 80kHz, 160kHz, 320kHz, 640kHz, 1.28MHz, 2MHz, Full).
Pulse Level High	Set the upper and lower pulse reference levels.
Pulse Level Low	
Next 2/2	Displays the first page of the menu


2.4 Configuring Sensor Input Voltage Measurements

Setting the Input Coupling (Coupling)

AC: Only displays the waveform produced from the input signal's AC component.

DC: Displays the waveform produced from both the DC and AC components of the input signal.


GND: Displays the ground level.

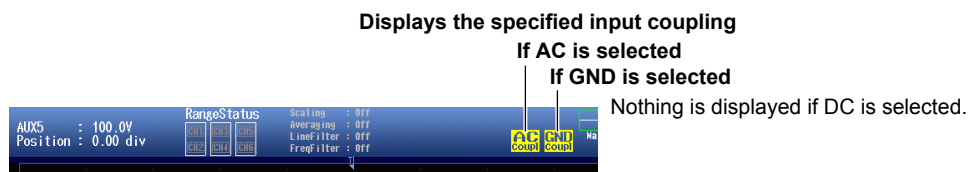

Input Coupling and Frequency Response

The frequency responses when the input coupling is set to AC and DC are shown below.

Note that the PX8000 does not acquire low-frequency signals or signal components if the input coupling is set to AC as indicated in the figure below.

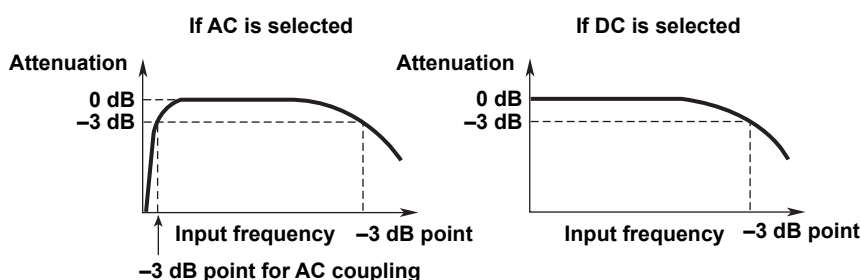

CAUTION

If the input coupling is AC, in accordance with the frequency response, the input signal is attenuated more in lower frequencies. As a result, even when a high voltage signal is actually applied, it may not be measured as a high voltage signal. Furthermore, the PEAK OVER message may not be displayed on the screen. As necessary, switch the input coupling to DC to check the input signal voltage.

Applying an input signal whose voltage exceeds the maximum input voltage of the AUX module may damage the input section.

Setting the Probe Attenuation (Probe)

1:1, 10:1, 100:1, 1000:1: Displays the voltage probe attenuation

Note

If the probe attenuation is not set correctly, the input signal voltage will not be displayed correctly. For example, if you use a 10:1 voltage probe but set the probe type to 1:1, the automatically measured amplitude of the waveform will be 1/10 the real value.

AUX Settings (Aux Settings)

Press the **Aux Settings** soft key to display the following screen.

When the input signal type is Analog

- When the linear scaling mode is AX+B

Set the input signal type to Analog.

The screenshot shows the 'Auxiliaries Settings' screen. The 'Sense Type' is set to 'Analog'. Under the 'Scaling' section, 'Scaling Mode' is set to 'AX+B'. The 'A' coefficient is set to '1.0000' and the 'B' offset is set to '0.0000'. The 'Unit String' field is empty. Under the 'Display Type' section, 'Mode' is set to 'Floating', 'Decimal Number' is set to 'Auto', and 'Sub Unit' is set to 'Auto'.

When the input signal type is Pulse

- When the linear scaling mode is AX+B

Set the input signal type to Pulse.

The screenshot shows the 'Auxiliaries Settings' screen. The 'Sense Type' is set to 'Pulse'. Under the 'Scaling' section, 'Scaling Mode' is set to 'AX+B'. The 'A' coefficient is set to '1.0000' and the 'B' offset is set to '0.0000'. The 'Unit String' field is empty. Under the 'Display Type' section, 'Mode' is set to 'Floating', 'Decimal Number' is set to 'Auto', and 'Sub Unit' is set to 'Auto'.

- When the linear scaling mode is P1-P2

Set the input signal type to Analog.

The screenshot shows the 'Auxiliaries Settings' screen. The 'Sense Type' is set to 'Analog'. Under the 'Scaling' section, 'Scaling Mode' is set to 'P1-P2'. Below this, there are four input fields for measured values: 'P1[X]' (1.0000), 'P1[Y]' (1.0000), 'P2[X]' (5.0000), and 'P2[Y]' (5.0000). Each field has a 'Get Value' button next to it. The 'Unit String' field is empty. Under the 'Display Type' section, 'Mode' is set to 'Floating', 'Decimal Number' is set to 'Auto', and 'Sub Unit' is set to 'Auto'.

- When the linear scaling mode is P1-P2

Set the input signal type to Pulse.

The screenshot shows the 'Auxiliaries Settings' screen. The 'Sense Type' is set to 'Pulse'. Under the 'Scaling' section, 'Scaling Mode' is set to 'P1-P2'. Below this, there are four input fields for measured values: 'P1[X]' (1.0000), 'P1[Y]' (1.0000), 'P2[X]' (5.0000), and 'P2[Y]' (5.0000). Each field has a 'Get Value' button next to it. The 'Unit String' field is empty. Under the 'Display Type' section, 'Mode' is set to 'Floating', 'Decimal Number' is set to 'Auto', and 'Sub Unit' is set to 'Auto'.

Setting the Sensor Input Voltage Measurement Range (Vertical Scale, RANGE Knob)

This section explains how to set a fixed range.

(If Auto Range in the AUX menu is set to ON, the measurement range changes depending on the amplitude of the input signal.)


Turn the **RANGE** knob to set the sensor input voltage measurement range.

- Auto Range in the AUX menu is set to OFF.
- If you turn the RANGE knob when waveform acquisition is stopped, two values are shown on the measurement range screen. The upper value is the measurement range for the displayed waveforms. The lower value is the measurement range that you have specified. The new range will be applied the next time waveform acquisition is started.
- If you do not operate the RANGE knob for approximately 3 seconds, the measurement range that you are setting with the knob will disappear from the screen.

Top row: Measurement range for the displayed waveforms

Bottom row: Measurement range that you have specified

When the displayed waveform's measurement range and the measurement range that you have set are the same, only the bottom row is displayed.



Use the **RANGE** knob to display the measurement range that is currently being set.

Measurement Range Options and Units

Below are the available options for the RANGE knob, measurement range values, and measurement range units that appear on the screen for when the zoom method is set to DIV and the zoom magnification is set to $\times 1$. If you change the zoom method or zoom magnification, what appears on the screen will change accordingly.

• When Waveform Acquisition Is Stopped

Input Signal Type	Linear Scaling Mode	Available Options for the RANGE Knob	Measurement Range Values (that appear on the screen)	Measurement Range Units (that appear on the screen)
Analog	OFF	(When the probe attenuation is 10:1) 500.0mV, 1.000V, 2.500V, 5.000V, 10.00V, 25.00V,	Upper value: RANGE knob value for the displayed waveform Lower value: Available option value of the RANGE knob	Upper unit value: Same unit as the available options for the RANGE knob Lower unit value: Same unit as the available options for the RANGE knob
	AX+B, P1–P2	50.00V, 100.0V, 250.0V, 500.0V, 1.000kV The available options vary depending on the probe attenuation setting.	Upper value: Value obtained by multiplying the available option value of the RANGE knob by the linear scaling coefficient. Lower value: Available option value of the RANGE knob	Upper unit value: Unit specified on the AUX setting screen Lower unit value: Same unit as the available options for the RANGE knob
Pulse	—	1, 2, 5, 10, 20, 50, 100, 200, 500, 1k, 2k, 5k, 10k, 20k, 50k, 100k, 200k, 500k, 1M	Upper value: No display Lower value: Available option value of the RANGE knob	Upper unit value: No display Lower unit value: Unit specified on the AUX setting screen


• When Waveform Acquisition Is Running

Input Signal Type	Linear Scaling Mode	Available Options for the RANGE Knob	Measurement Range Values (that appear on the screen)	Measurement Range Units (that appear on the screen)
Analog	OFF	(When the probe attenuation is 10:1) 500.0mV, 1.000V, 2.500V, 5.000V,	Upper value: No display Lower value: Available option value of the RANGE knob	Upper unit value: No display Lower unit value: Same unit as the available options for the RANGE knob
	AX+B, P1–P2	10.00V, 25.00V, 50.00V, 100.0V, 250.0V, 500.0V, 1.000kV The available options vary depending on the probe attenuation setting.	Upper value: Value obtained by multiplying the available option value of the RANGE knob by the linear scaling coefficient. Lower value: Available option value of the RANGE knob	Upper unit value: Unit specified on the AUX setting screen Lower unit value: Same unit as the available options for the RANGE knob
Pulse	—	1, 2, 5, 10, 20, 50, 100, 200, 500, 1k, 2k, 5k, 10k, 20k, 50k, 100k, 200k, 500k, 1M	Upper value: No display Lower value: Available option value of the RANGE knob	Upper unit value: No display Lower unit value: Unit specified on the AUX setting screen

Setting the Sensor Input Voltage Waveform Vertical Position When the Zoom Method is Set to DIV (Vertical POSITION Knob)


Turn the **vertical POSITION** knob to set the waveform vertical position.

- Set in the range of –5.00 div to 5.00 div.
- If you do not operate the vertical POSITION knob for approximately 3 seconds, the vertical position that you are setting with the knob will disappear from the screen.

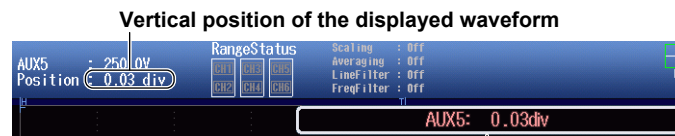

Use the vertical **POSITION** knob to display the vertical position that is currently being set.

- You can set the vertical position to 0 div by pressing the knob.



This indicates that you can press the vertical **POSITION** knob to set the vertical position to 0 div.

When the Zoom Method is Set to SPAN (Upper and Lower Limits)

Using the **Upper/Lower** soft key and the **jog shuttle**, set the voltage at the top edge of the waveform screen (upper limit) and the voltage at the bottom edge of the screen (lower limit) to set the waveform vertical position.

AUX5 (CH5)	
Display	
OFF	ON
Label	
AUX5	
Vertical Scale	
DIV	SPAN
Upper	250.0V
Lower	-250.0V
Auto Range	
OFF	ON
Aux Settings (Analog/Pulse)	
Analog	
Next 1/2	

Set the upper and lower limits of the display range.

2.5 Configuring Rotating Speed Measurements

This section explains the following settings for the vertical axis of rotating speed measurements.

- Waveform display on and off
- Display labels
- Zoom method
 - DIV: Magnification for zooming waveforms, offset
 - SPAN: Upper and lower display limits for zooming waveforms
- Auto range on and off
- Rotating speed measurement
 - Input signal type, linear scaling, display format
- Input coupling
- Bandwidth limit
- Upper and lower pulse reference levels
- Rotating speed measurement range
- Rotating speed waveform vertical position

► [Features Guide: “Sensor Input Voltage Measurement \(AUX\)”](#)
[“Rotating Speed Settings \(Speed Settings\)”](#)

Check that an AUX module is installed in slot 3, 5, or 7.

Pm Menu

Of the **ELEM 2 to ELEM 4** keys, press the key corresponding to the slot in which the AUX module is installed. On the menu that appears, set Motor Mode to ON.

Pm3	
Motor Mode	
OFF	ON
Name	
Pm3	
Scaling	
1.0000	
Unit	
W	
Sync Source	
None	

Set Motor Mode to ON.

Set the function name.

Set the scaling coefficient.

Set the unit.

Set the synchronization source. ► [section 1.3](#)

AUX Menu

- Press **U2(CH3)**, **U3(CH5)**, or **U4(CH7)** to select a channel on an installed AUX module. The following menu appears.

When the zoom method is set to **DIV**

Display OFF ON	Turns the waveform display on and off
Label AUX5	Set the display label.
Vertical Scale DIV SPAN	Set the zoom method to DIV.
Vertical Zoom x 1	Set the zoom magnification.
Offset 0.00rpm	Set the offset.
Auto Range OFF ON	Turns the auto range on and off*
Speed Settings (Analog/Pulse) Analog	Configure rotating speed measurement.
Next 1/2	Displays the second page of the menu

When the zoom method is set to **SPAN**

Display OFF ON	Turns the waveform display on and off
Label AUX5	Set the display label.
Vertical Scale DIV SPAN	Set the zoom method to SPAN.
Upper 25.00rpm Lower -25.00rpm	Set the upper and lower limits of the display range.
Auto Range OFF ON	Turns the auto range on and off*
Speed Settings (Analog/Pulse) Analog	Configure rotating speed measurement.
Next 1/2	Displays the second page of the menu

* You can turn auto range on and off when the rotating-speed input signal type is set to Analog. If the type is set to Pulse, auto range is fixed to OFF.

Note

The U key whose display setting is ON illuminates. If the U key is not illuminated, you can press it to turn on the waveform display and the key. If the U key is illuminated, you can press it to turn off the waveform display and the key.

- Press the **Next 1/2** soft key to display the 2/2 menu.

When the rotating-speed input signal type is **Analog**

Coupling DC	Set the input coupling (AC, DC, GND).
Probe Full	
Bandwidth Full	Set the bandwidth limit (10kHz, 20kHz, 40kHz, 80kHz, 160kHz, 320kHz, 640kHz, 1.28MHz, 2MHz, Full).
Pulse Level High 2.4V	
Pulse Level Low 0.4V	
Next 2/2	Displays the first page of the menu

When the rotating-speed input signal type is **Pulse**

Coupling DC	
Probe Full	Set the bandwidth limit (10kHz, 20kHz, 40kHz, 80kHz, 160kHz, 320kHz, 640kHz, 1.28MHz, 2MHz, Full).
Pulse Level High 2.4V	Set the upper and lower pulse reference levels.
Pulse Level Low 0.4V	
Next 2/2	Displays the first page of the menu

Setting the Input Coupling (Coupling)

This is the same feature as the input coupling of sensor input voltage measurement. ► [section 2.4](#)

Configuring Rotating Speed Measurements (Speed Settings)

Press the **Speed Settings** soft key to display the following screen.

When the input signal type is Analog

- When the linear scaling mode is AX+B

The screenshot shows the 'Motor Speed Settings' screen. The 'Sense Type' is set to 'Analog'. The 'Unit' is set to 'rpm'. Under the 'Analog' section, 'Scaling Mode' is set to 'AX+B'. The 'A' coefficient is '1.000' and the 'B' offset is '0.0000'. Under the 'Display Type' section, 'Mode' is set to 'Floating', 'Decimal Number' is 'Auto', and 'Sub Unit' is 'Auto'. Callouts point to these settings with instructions: 'Set the input signal type to Analog.', 'Select the rotating speed unit (rps, rpm, rph).', 'Set the linear scaling mode to AX+B.', 'Set the scaling coefficient.', 'Set the offset.', 'Select the display mode.', 'Select the number of decimal places.', and 'Select the unit prefix.'

- When the linear scaling mode is P1-P2

The screenshot shows the 'Motor Speed Settings' screen with 'Scaling Mode' set to 'P1-P2'. It includes fields for 'P1[X]', 'P1[Y]', 'P2[X]', and 'P2[Y]', each with a 'Get Value' button. The 'Display Type' section is identical to the previous screen. Callouts provide instructions: 'Set the input signal type to Analog.', 'Select the rotating speed unit (rps, rpm, rph).', 'Set the linear scaling mode P1-P2.', 'Retrieve the current measured values.', 'Set the measured values.', 'Set the scale values.', and 'Same feature as when linear scaling mode is set to AX+B'.

When the input signal type is Pulse

The screenshot shows the 'Motor Speed Settings' screen with 'Sense Type' set to 'Pulse'. The 'Unit' is 'rpm'. Under the 'Pulse' section, 'Pulse N' is set to '60' with the unit 'Pulses/Revolution'. The 'Display Type' section is identical to the previous screens. Callouts provide instructions: 'Set the input signal type to Pulse.', 'Select the rotating speed unit (rps, rpm, rph).', 'Set the number of pulses per rotation (1-9999).', and 'Same feature as when the input signal type is set to Analog'.

Setting the Rotating Speed Measurement Range (Vertical Scale, RANGE Knob)

This section explains how to set a fixed range.


(If Auto Range in the AUX menu is set to ON, the measurement range changes depending on the amplitude of the input signal.)

Turn the **RANGE** knob to set the rotating speed measurement range.

- Auto Range in the AUX menu is set to OFF.
- If the input signal type is analog and you turn the RANGE knob when waveform acquisition is stopped, two values are shown on the measurement range screen. The upper value is the measurement range for the displayed waveforms. The lower value is the measurement range that you have specified. The new range will be applied the next time waveform acquisition is started.
- If you do not operate the RANGE knob for approximately 3 seconds, the measurement range that you are setting with the knob will disappear from the screen.

Top row: Measurement range for the displayed waveforms

Bottom row: Measurement range that you have specified



Use the **RANGE** knob to display the measurement range that is currently being set.

Measurement Range Options and Units

Below are the available options for the RANGE knob, measurement range values, and measurement range units that appear on the screen for when the zoom method is set to DIV and the zoom magnification is set to $\times 1$. If you change the zoom method or zoom magnification, what appears on the screen will change accordingly.

• When Waveform Acquisition Is Stopped

Input Signal Type	Linear Scaling Mode	Available Options for the RANGE Knob	Measurement Range Values (that appear on the screen)	Measurement Range Units (that appear on the screen)
Analog	OFF	50.00mV, 100.0mV, 250.0mV, 500.0mV, 1.000V, 2.500V, 5.000V,	Upper value: RANGE knob value for the displayed waveform Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the rotating speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
	AX+B, P1-P2	10.00V, 25.00V, 50.00V, 100.0V	Upper value: Value obtained by multiplying the available option value of the RANGE knob by the linear scaling coefficient. Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the rotating speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
Pulse	—	1, 2, 5, 10, 20, 50, 100, 200, 500, 1k, 2k, 5k, 10k, 20k, 50k, 100k, 200k, 500k, 1M	Upper value: No display Lower value: Available option value of the RANGE knob	Upper unit value: No display Lower unit value: Unit selected on the rotating speed measurement setting screen

• When Waveform Acquisition Is Running

Input Signal Type	Linear Scaling Mode	Available Options for the RANGE Knob	Measurement Range Values (that appear on the screen)	Measurement Range Units (that appear on the screen)
Analog	OFF	50.00mV, 100.0mV, 250.0mV, 500.0mV, 1.000V, 2.500V, 5.000V,	Upper value: Available option value of the RANGE knob Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the rotating speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
	AX+B, P1–P2	10.00V, 25.00V, 50.00V, 100.0V	Upper value: Value obtained by multiplying the available option value of the RANGE knob by the linear scaling coefficient. Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the rotating speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
Pulse	—	1, 2, 5, 10, 20, 50, 100, 200, 500, 1k, 2k, 5k, 10k, 20k, 50k, 100k, 200k, 500k, 1M	Upper value: No display Lower value: Available option value of the RANGE knob	Upper unit value: No display Lower unit value: Unit selected on the rotating speed measurement setting screen

Setting the Rotating Speed Waveform Vertical Position

When the Zoom Method is Set to DIV (Vertical POSITION Knob)

Turn the **vertical POSITION** knob to set the waveform vertical position.


- Set in the range of –5.00 div to 5.00 div.
- If you do not operate the vertical POSITION knob for approximately 3 seconds, the vertical position that you are setting with the knob will disappear from the screen.

Vertical position of the displayed waveform



Use the vertical **POSITION** knob to display the vertical position that is currently being set.

- You can set the vertical position to 0 div by pressing the knob.



RANGE knob


Vertical **POSITION** knob

This indicates that you can press the vertical **POSITION** knob to set the vertical position to 0 div.

2.5 Configuring Rotating Speed Measurements

When the Zoom Method is Set to SPAN (Upper and Lower Limits)

Using the **Upper/Lower** soft key and the **jog shuttle**, set the number of rotations at the top edge of the waveform screen (upper limit) and the number of rotations at the bottom edge of the screen (lower limit) to set the waveform vertical position.

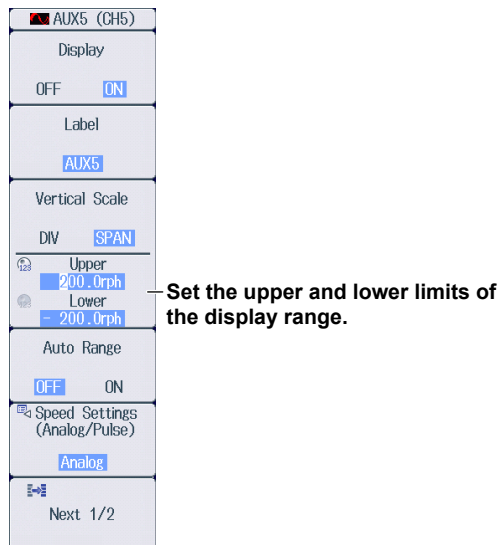

2.6 Configuring Torque Measurements

This section explains the following settings for the vertical axis of torque measurements.

- Waveform display on and off
- Display labels
- Zoom method
 - DIV: Magnification for zooming waveforms, offset
 - SPAN: Upper and lower display limits for zooming waveforms
- Auto range on and off
- Torque measurement
 - Input signal type, linear scaling, display format
- Input coupling
- Bandwidth limit
- Upper and lower pulse reference levels
- Torque measurement range
- Torque waveform vertical position

► [Features Guide: “Sensor Input Voltage Measurement \(AUX\)”](#)
“Torque Settings (Torque Settings)”

Check that an AUX module is installed in slot 3, 5, or 7.

Pm Menu

Of the **ELEM 2** to **ELEM 4** keys, press the key corresponding to the slot in which the AUX module is installed. On the menu that appears, set Motor Mode to ON.

Pm3	
Motor Mode	
OFF	ON
Name	
Pm3	
Scaling	
1.0000	
Unit	
W	
Sync Source	
None	

Set Motor Mode to ON.

Set the function name.

Set the scaling coefficient.


Set the unit.

Set the synchronization source. ► [section 1.3](#)


AUX Menu

- Press **I2(CH4)**, **I3(CH6)**, or **I4(CH8)** to select a channel on an installed AUX module. The following menu appears.

When the zoom method is set to DIV

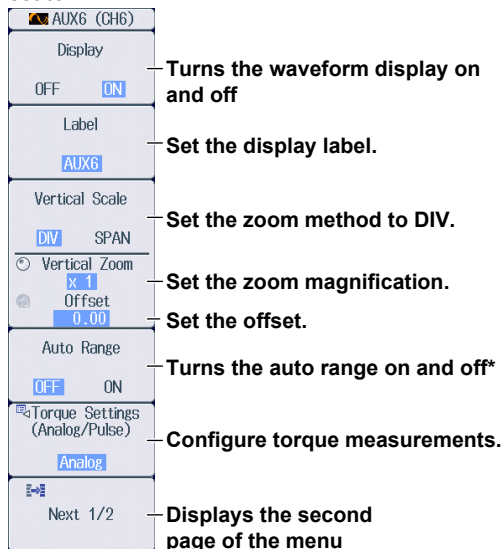

When the zoom method is set to SPAN

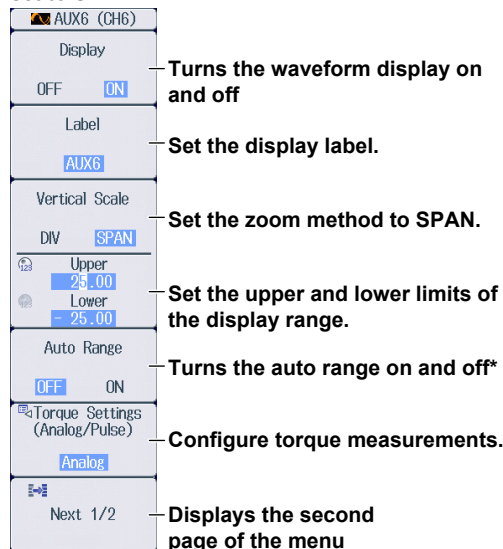


* You can turn auto range on and off when the torque input signal type is set to Analog. If the type is set to Pulse, auto range is fixed to OFF.

Note


The I key whose display setting is ON illuminates. If the I key is not illuminated, you can press it to turn on the waveform display and the key. If the I key is illuminated, you can press it to turn off the waveform display and the key.

- Press the **Next 1/2** soft key to display the 2/2 menu.

When the torque input signal type is Analog

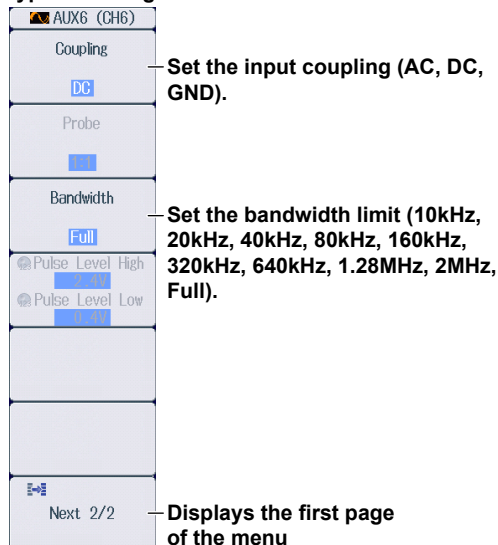

When the torque input signal type is Pulse

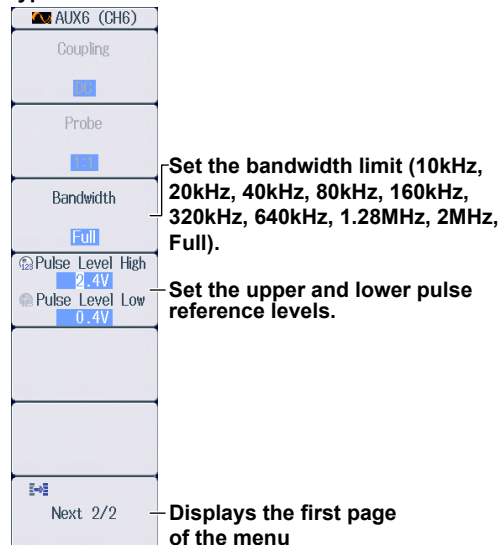

Setting the Input Coupling (Coupling)

This is the same feature as the input coupling of sensor input voltage measurement. ► [section 2.4](#)

Configuring Torque Measurements (Torque Settings)

Press the **Torque Settings** soft key to display the following screen.

When the input signal type is Analog

- When the linear scaling mode is AX+B

The screenshot shows the 'Motor Torque Settings' screen. The 'Sense Type' is set to 'Analog'. The 'Unit' field is empty. Under the 'Analog' section, 'Scaling Mode' is set to 'AX+B'. The 'A' coefficient is 1.0000 and the 'B' offset is 0.0000. Under the 'Display Type' section, 'Mode' is 'Floating', 'Decimal Number' is 'Auto', and 'Sub Unit' is 'Auto'. Callouts on the right point to these settings with instructions.

- When the linear scaling mode is P1-P2

The screenshot shows the 'Motor Torque Settings' screen with 'Scaling Mode' set to 'P1-P2'. It includes fields for 'P1[X]', 'P1[Y]', 'P2[X]', and 'P2[Y]', each with a 'Get Value' button. The 'Display Type' section is identical to the previous screen. Callouts on the right provide instructions for each field.

When the input signal type is Pulse

The screenshot shows the 'Motor Torque Settings' screen with 'Sense Type' set to 'Pulse'. The 'Unit' field is empty. Under the 'Pulse' section, 'Rated Upper' is 50.0000 and 'Rated Lower' is -50.0000. To the right, there are fields for pulse frequencies: 15000Hz and 5000Hz. The 'Display Type' section is identical to the previous screens. Callouts on the right provide instructions.

Setting the Torque Measurement Range (Vertical Scale, RANGE Knob)

This section explains how to set a fixed range.


(If Auto Range in the AUX menu is set to ON, the measurement range changes depending on the amplitude of the input signal.)

Turn the **RANGE** knob to set the torque measurement range.

- Auto Range in the AUX menu is set to OFF.
- If the input signal type is analog and you turn the RANGE knob when waveform acquisition is stopped, two values are shown on the measurement range screen. The upper value is the measurement range for the displayed waveforms. The lower value is the measurement range that you have specified. The new range will be applied the next time waveform acquisition is started.
- If you do not operate the RANGE knob for approximately 3 seconds, the measurement range that you are setting with the knob will disappear from the screen.

Top row: Measurement range for the displayed waveforms

Bottom row: Measurement range that you have specified



Use the **RANGE** knob to display the measurement range that is currently being set.

Measurement Range Options and Units

Below are the available options for the RANGE knob, measurement range values, and measurement range units that appear on the screen for when the zoom method is set to DIV and the zoom magnification is set to $\times 1$. If you change the zoom method or zoom magnification, what appears on the screen will change accordingly.

• When Waveform Acquisition Is Stopped

Input Signal Type	Linear Scaling Mode	Available Options for the RANGE Knob	Measurement Range Values (that appear on the screen)	Measurement Range Units (that appear on the screen)
Analog	OFF	50.00mV, 100.0mV, 250.0mV, 500.0mV, 1.000V, 2.500V,	Upper value: RANGE knob value for the displayed waveform Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the torque speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
	AX+B, P1-P2	5.000V, 10.00V, 25.00V, 50.00V, 100.0V	Upper value: Value obtained by multiplying the available option value of the RANGE knob by the linear scaling coefficient. Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the torque speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
Pulse	—	1, 2, 5, 10, 20, 50, 100, 200, 500, 1k, 2k, 5k, 10k, 20k, 50k, 100k, 200k, 500k, 1M	Upper value: No display Lower value: Available option value of the RANGE knob	Upper unit value: No display Lower unit value: Unit selected on the torque speed measurement setting screen

- When Waveform Acquisition Is Running

Input Signal Type	Linear Scaling Mode	Available Options for the RANGE Knob	Measurement Range Values (that appear on the screen)	Measurement Range Units (that appear on the screen)
Analog	OFF	50.00mV, 100.0mV, 250.0mV, 500.0mV, 1.000V, 2.500V,	Upper value: Available option value of the RANGE knob Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the torque speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
	AX+B, P1–P2	5.000V, 10.00V, 25.00V, 50.00V, 100.0V	Upper value: Value obtained by multiplying the available option value of the RANGE knob by the linear scaling coefficient. Lower value: Available option value of the RANGE knob	Upper unit value: Unit selected on the torque speed measurement setting screen Lower unit value: Same unit as the available options for the RANGE knob
Pulse	—	1, 2, 5, 10, 20, 50, 100, 200, 500, 1k, 2k, 5k, 10k, 20k, 50k, 100k, 200k, 500k, 1M	Upper value: No display Lower value: Available option value of the RANGE knob	Upper unit value: No display Lower unit value: Unit selected on the torque speed measurement setting screen


Setting the Torque Waveform Vertical Position

When the Zoom Method is Set to DIV (Vertical POSITION Knob)

Turn the **vertical POSITION** knob to set the waveform vertical position.


- Set in the range of –5.00 div to 5.00 div.
- If you do not operate the vertical POSITION knob for approximately 3 seconds, the vertical position that you are setting with the knob will disappear from the screen.

Vertical position of the displayed waveform



Use the vertical **POSITION** knob to display the vertical position that is currently being set.

- You can set the vertical position to 0 div by pressing the knob.




RANGE knob

Vertical POSITION knob

This indicates that you can press the vertical POSITION knob to set the vertical position to 0 div.

When the Zoom Method is Set to SPAN (Upper and Lower Limits)

Using the **Upper/Lower** soft key and the **jog shuttle**, set the torque at the top edge of the waveform screen (upper limit) and the torque at the bottom edge of the screen (lower limit) to set the waveform vertical position.

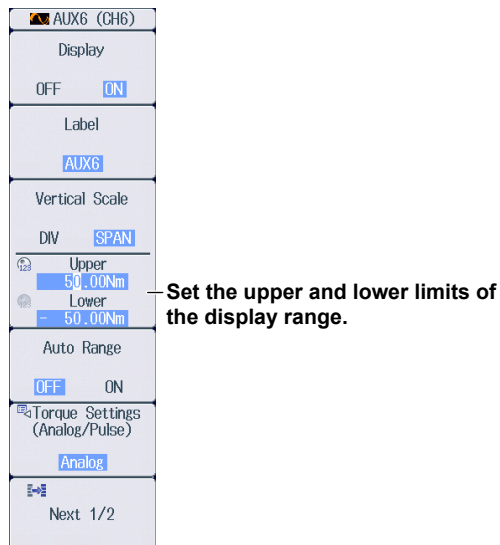

2.7 Displaying the Menu for Configuring All Channels

This section explains the following settings for configuring all channels.


- Settings of all elements
- Settings of all AUX channels
- Copying setup data

► **Features Guide: “Displaying the Menu for Configuring All Channels (ALL CH)”**


ALL CH menu

Press **ALL CH** to display the following menu.

Displaying the settings of all elements

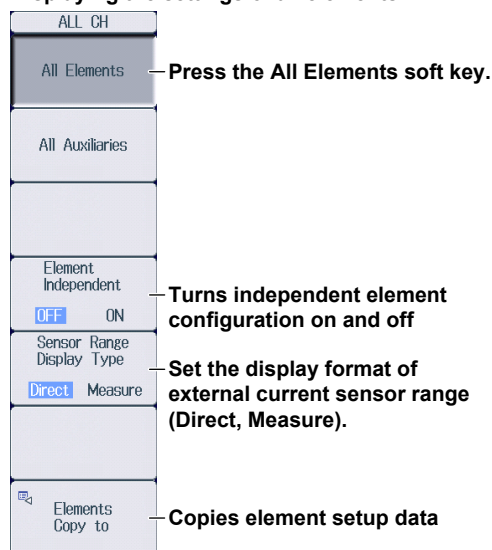

Displaying the settings of all AUX channels

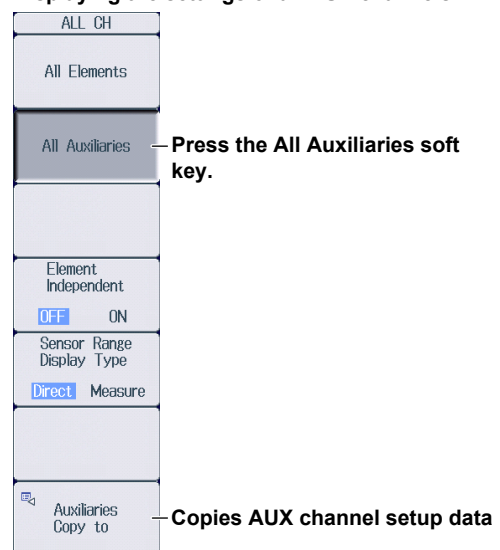

Settings of All Elements (All Elements)

1. Press the **All Elements** soft key to display the following screen.

Use the **jog shuttle** to select the setting that you want to change, and then press **SET** to display the available options or an input box.

To set all elements to the same setting at once, change the settings in the All column.

All Elements Setup				
All	Element 1	Element 2		
Wiring	1P2W	1P2W		
U Auto Range	OFF	OFF		
U Range	100V	100V		
Ext Sensor	OFF	OFF		
I Auto Range	OFF	OFF		
I Range	5A	5A		
Sensor Ratio	10.0000 mV/A	10.0000 mV/A		
Coupling	DC	DC		
Scaling	OFF	OFF		
VT Scaling	1.0000	1.0000		
CT Scaling	1.0000	1.0000		
SF Scaling	1.0000	1.0000		
Sync Source	I1	I2		
Line Filter	OFF	OFF		
Freq Filter	OFF	OFF		

Use the **jog shuttle** to select the item that you want to set.

2.7 Displaying the Menu for Configuring All Channels

Copying Element Setup Data (Elements Copy to)

2. Press the **Elements Copy to** soft key to display the following screen.

Copy to

Source:

Destination:

☐ Element 1

☒ Element 2

Annotations:

- Set the copy source element.
- Selects all elements except the copy source to be copy destinations
- Clears all elements from being copy destinations
- Select the element check boxes separately to set the copy destination.
- Starts copying

Settings of All AUX Channels

1. Press the **All Auxiliaries** soft key to display the following screen.

Use the **jog shuttle** to select the setting that you want to change, and then press **SET** to display the available options or an input box.

	CH5 AUX 5	CH6 AUX 6				
Motor Mode	OFF					
Pm Name	Pm3					
Pm Scaling	1.0000					
Pm Unit	W					
Sync Source	None					
Sense Type	Analog	Analog				
Unit						
Auto Range	OFF	OFF				
Range	250V	250V				
Scaling Mode	OFF	OFF				
A	1.0000	1.0000				
B	0.0000	0.0000				
P1[X]	1.0000	1.0000				
P1[Y]	1.0000	1.0000				
P2[X]	5.0000	5.0000				
P2[Y]	5.0000	5.0000				
Pulse N	60					
Rated Upper		50.0000				
Rated Freq Upper		15000Hz				
Rated Lower		-50.0000				
Rated Freq Lower		5000Hz				
Bandwidth	Full	Full				
Coupling	DC	DC				
Probe	10:1	10:1				
Pulse Level High	2.4V	2.4V				
Pulse Level Low	0.4V	0.4V				

Use the jog shuttle to select the item that you want to set.

Copying AUX Channel Setup Data (Auxiliaries Copy to)

2. Press the **Auxiliaries Copy to** soft key to display the following screen.

Copy to

Source:

Destination:

☐ AUX5 ☒ AUX6

Annotations:

- Set the copy source channel.
- Selects all channels except the copy source to be copy destinations
- Clears all channels from being copy destinations
- Select the channel check boxes separately to set the copy destination.
- Starts copying


2.8 Configuring the Horizontal Axis (Time axis)

This section explains how to set the time scale (the time per grid (1 div) displayed on the screen).

► [Features Guide: “Horizontal Axis”](#)


Configuring the Horizontal Axis (Time axis)

Turn the **TIME/DIV** knob to set the time scale.

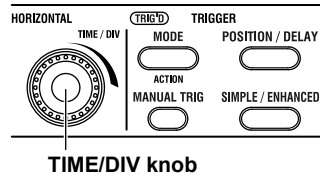

Time Scale (TIME/DIV) Display

- If you turn the TIME/DIV knob when waveform acquisition is stopped, the time scale display shows the time scale for the currently displayed waveform in the upper row and the changed time scale in the lower row. The new time scale will be applied the next time waveform acquisition is started.
- If you do not operate the TIME/DIV knob for approximately 3 seconds, the time scale that you are setting with the knob will disappear from the screen.

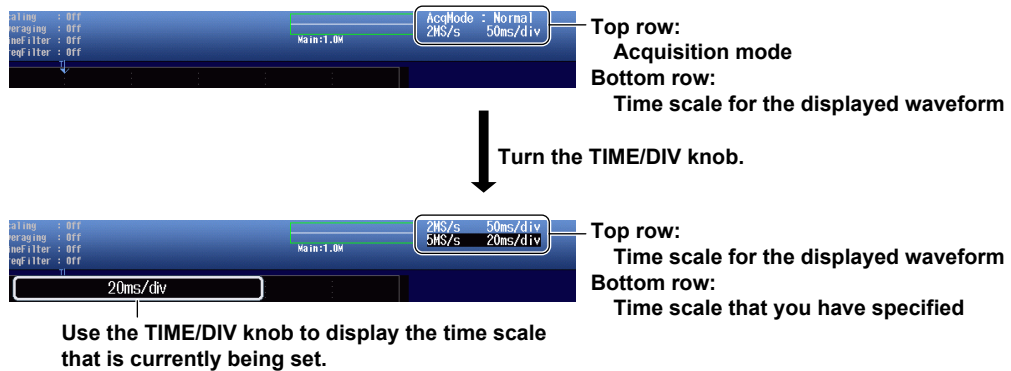

3.1 Setting the Trigger Mode


This section explains the following setting for updating the displayed waveform.

- Trigger mode

► [Features Guide: “Trigger Mode \(MODE\)”](#)

MODE menu

Press **MODE** to display the following menu.

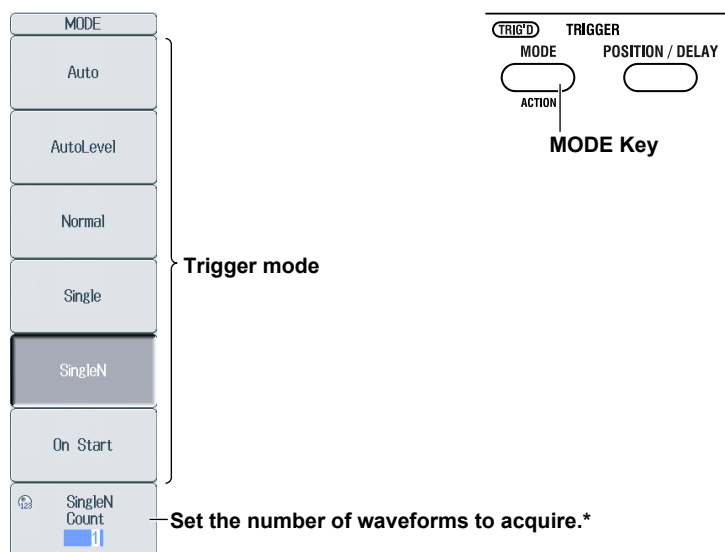

* Displayed when the trigger mode is set to SingleN.

Setting the Trigger Mode (Mode)

- Auto:** If the trigger conditions are met within 50 ms, the PX8000 updates the displayed waveforms on each trigger occurrence. If not, the PX8000 automatically updates the displayed waveforms. If the time axis is set to a value that would cause the display to switch to roll mode, the roll mode display will be enabled.
- AutoLevel:** If a trigger occurs before a timeout (which is approximately 1 second), the PX8000 updates the waveform in the same way that it does in Auto mode. If a trigger does not occur before a timeout, the PX8000 automatically changes the trigger level to the center value of the trigger source amplitude, triggers on that value, and updates the displayed waveform.
- Normal:** The PX8000 only updates the waveform display when the trigger conditions are met.
- Single:** When the trigger conditions are met, the PX8000 updates the displayed waveform once and stops signal acquisition. If the time axis is set to a value that would cause the display to switch to roll mode, the roll mode display will be enabled. When the PX8000 triggers, it begins recording data. When data has been acquired up to the amount specified by the set record length, the waveform display stops.
- SingleN:** The PX8000 acquires signals each time the trigger conditions are met until a specified number of signals have been acquired, and then displays all of the acquired signals. If no triggers occur, the display is not updated.
- On Start:** Regardless of the trigger settings, when you press the START key, the PX8000 updates the displayed waveforms once and stops signal acquisition. If the time axis is set to a value that would cause the display to switch to roll mode, the roll mode display will be enabled. When data has been acquired up to the amount specified by the set record length, the waveform display stops.

3.2 Setting the Trigger Position and Trigger Delay



This section explains the following settings for updating the displayed waveform.

- Trigger position
- Trigger delay

► [Features Guide: “Trigger Position \(Position\)”](#)
[“Trigger Delay \(Delay\)”](#)

POSITION/DELAY Menu

Press **POSITION/DELAY** to display the following menu.

POSITION/DELAY	
 Position 50.0%	Set the trigger position.
Set to 10%	Set the trigger position to 10%.
Set to 50%	Set the trigger position to 50%.
Set to 90%	Set the trigger position to 90%.
 Delay 0.00us	Set the trigger delay.

3.3 Setting the Trigger Hold Off


This section explains the following setting for updating the displayed waveform.

- Hold-off time

► [Features Guide: “Trigger Hold Off \(Hold Off\)”](#)

SIMPLE/ENHANCED Menu

Press **SIMPLE/ENHANCED** to display the following menu.

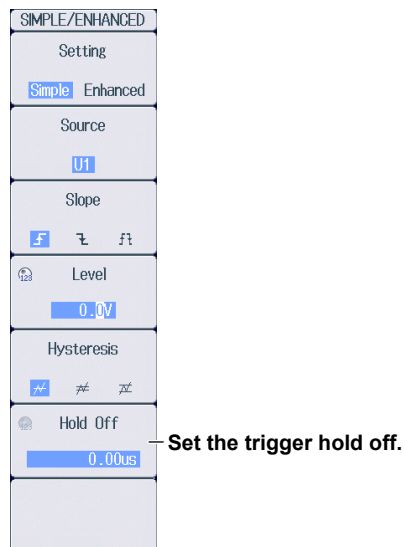

Setting the Hold-off Time (Hold Off)

The trigger hold-off feature temporarily stops the detection of the next trigger once a trigger has occurred.

3.4 Triggering on an Edge Trigger (Simple)


This section explains the following settings for triggering on the edges of a signal applied to an installed module.

- Trigger source
- Trigger slope
- Trigger level
- Trigger hysteresis

► **Features Guide:** “Simple Trigger (Simple),” “Trigger Source (Source),” “Trigger Slope (Slope),” “Trigger Level (Level),” and “Trigger Hysteresis (Hysteresis)”

SIMPLE Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Simple. The following menu appears.

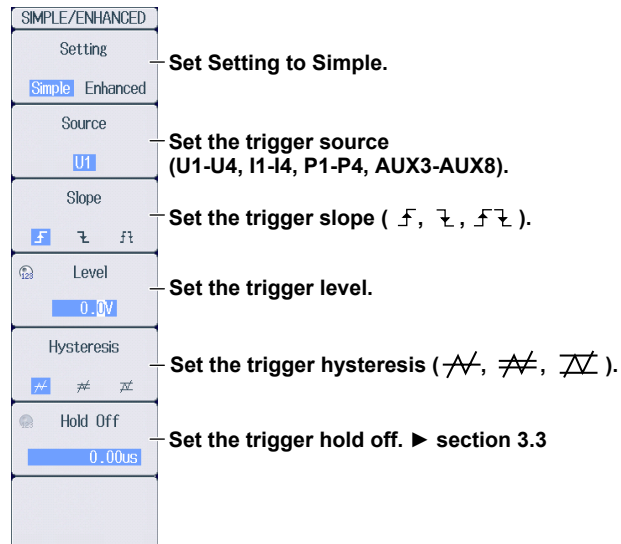


3.5 Triggering on a Timer Trigger (Simple)

This section explains the settings that are used when triggering on a specific date and time.

► [Features Guide: “Time \(Time\)”](#)

SIMPLE Time Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Simple. The following menu appears.

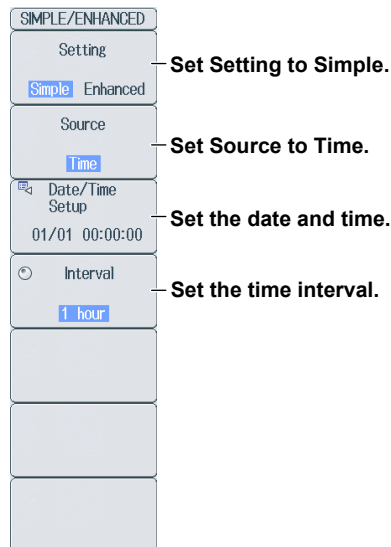


The screenshot shows a vertical menu with the following options and annotations:

- SIMPLE/ENHANCED** (header)
- Setting** (with **Simple** and **Enhanced** sub-options) — **Set Setting to Simple.**
- Source** (with **Time** sub-option) — **Set Source to Time.**
- Date/Time Setup** (with **01/01 00:00:00**) — **Set the date and time.**
- Interval** (with **1 hour**) — **Set the time interval.**
- Three empty menu items at the bottom.

Setting the Date and Time (Date/Time Setup)

Press the **Date/Time Setup** soft key to display the following screen.

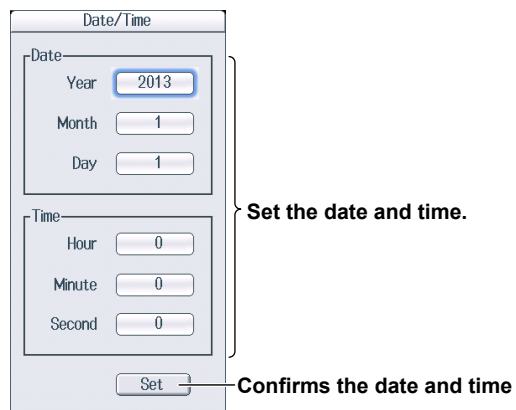

The screenshot shows the **Date/Time Setup** screen with the following fields and annotations:

- Date/Time** (header)
- Date** section:
 - Year**: 2013
 - Month**: 1
 - Day**: 1
- Time** section:
 - Hour**: 0
 - Minute**: 0
 - Second**: 0
- Set** button — **Confirms the date and time**

A bracket on the right side of the Date and Time sections indicates: **Set the date and time.**


3.6 Triggering on an External Trigger (Simple)

This section explains the settings that are used when triggering on an external signal.

► [Features Guide: “External Signal \(External\)”](#)
“Trigger Slope (Slope)”

SIMPLE External Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Simple. The following menu appears.

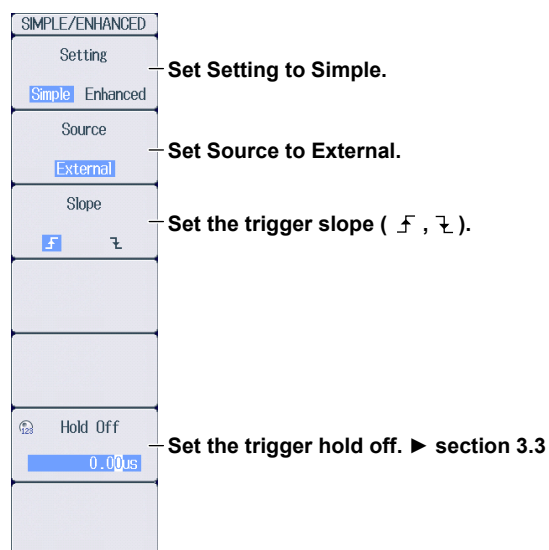


3.7 Triggering on a Power Line Signal (Simple)

This section explains the settings that are used when triggering on a power line signal.

► [Features Guide: “Power Line Signal \(Line\)”](#)

SIMPLE Line Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Simple. The following menu appears.

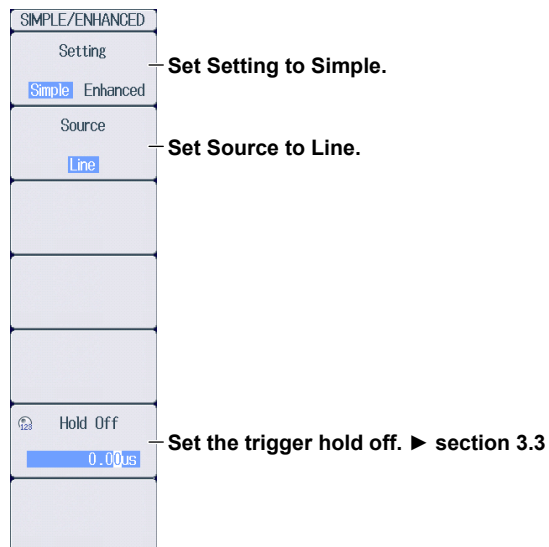

3.8 Triggering on an A -> B(N) Trigger (Enhanced)

This section explains the following settings for triggering on an A -> B(N) trigger.

- Trigger source
- State condition
- State condition achievement condition
- Number of times state condition B must be met
- Trigger condition

► [Features Guide: “A -> B\(N\) Trigger \(Enhanced\)”](#)

ENHANCED_A->B(N) Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

SIMPLE/ENHANCED

Setting

Simple **Enhanced**

Type

A -> B(N)

Set Pattern

Hold Off

0.00us

Setting the State and Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

Set the state condition (H, L, or X (do not use as a trigger source)).

Set the trigger level.

Set the hysteresis (∇ , ∇ , ∇).

	A State	B State	Level	Hys
U1	H	H	0.0V	∇
I1	X	X	0.00A	∇
P1	X	X	0W	∇
U2	X	X	0.0V	∇
I2	X	X	0.00A	∇
P2	X	X	0W	∇
AUX5	X	X	0.0V	∇
AUX6	X	X	0.0V	∇

A Condition

Enter Exit

B Condition

Enter Exit

Count

1

Set the state condition achievement conditions (Enter, Exit).

Set the number of times state condition B must be met.

Met Met N times

A → B B → Trigger

3.9 Triggering on an A Delay B Trigger (Enhanced)

This section explains the following settings for triggering on an A Delay B trigger.

- Trigger source
- State condition
- State condition achievement condition
- Delay time
- Trigger condition

► [Features Guide: “A Delay B Trigger \(Enhanced\)”](#)

ENHANCED A Delay B Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

The screenshot shows a vertical menu with the following options and annotations:

- SIMPLE/ENHANCED**: Header of the menu.
- Setting**: Sub-header.
- Simple** and **Enhanced**: Two buttons. **Enhanced** is highlighted. Annotation: **Set Setting to Enhanced.**
- Type**: Sub-header.
- A Delay B**: A button. Annotation: **Set Type to A Delay B.**
- Set Pattern**: A button. Annotation: **Set the state and trigger conditions.**
- Hold Off**: A sub-header.
- 0.00us**: A value field. Annotation: **Set the trigger hold off. ► section 3.3**

Setting the State and Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

The screenshot shows the **Set Pattern** menu with the following elements and annotations:

- A Delay B**: Header of the menu.
- A State**, **B State**, **Level**, **Hys**: Columns in the table.
- U1**, **I1**, **P1**, **U2**, **I2**, **P2**, **AUX5**, **AUX6**: Rows in the table.
- Set the state condition (H, L, or X (do not use as a trigger source)).**: Annotation pointing to the A State column.
- Set the trigger level.**: Annotation pointing to the Level column.
- Set the hysteresis (\overline{A} , \overline{B} , $\overline{A/B}$).**: Annotation pointing to the Hys column.
- A Condition**: Sub-header.
- Enter** and **Exit**: Buttons.
- B Condition**: Sub-header.
- Enter** and **Exit**: Buttons.
- Set the state condition achievement conditions (Enter, Exit).**: Annotation pointing to the Enter/Exit buttons.
- Delay**: Sub-header.
- 0.00us**: A value field.
- Set the delay time.**: Annotation pointing to the Delay field.
- Met**: A label.
- A**: A box.
- Delay time passes**: A box.
- B**: A box.
- Trigger**: A label.

The diagram at the bottom shows the flow: **Met A** → **Delay time passes** → **Met B** → **Trigger**.

3.10 Triggering on an Edge On A Trigger (Enhanced)

This section explains the following settings for triggering on an Edge On A trigger.

- Trigger source
- State condition
- State condition achievement condition
- Edge detection condition
- Trigger condition

► [Features Guide: “Edge On A Trigger \(Enhanced\)”](#)

ENHANCED Edge On A Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

SIMPLE/ENHANCED

Setting
Simple **Enhanced** — **Set Setting to Enhanced.**

Type
Edge On A — **Set Type to Edge On A.**

Set Pattern — **Set the state and trigger conditions.**

Hold Off
0.00us — **Set the trigger hold off. ► section 3.3**

Setting the State and Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

Set the state condition (H, L, or X (do not use as a trigger source)).

Set the edge detection condition (\uparrow , \downarrow , \rightarrow).

Set the trigger level.

Set the hysteresis (\swarrow , \searrow , \nwarrow).

Set the state condition achievement conditions (True, False).

	A State	Edge	Level	Hys	Condition
U1	H	—	0.0V	\swarrow	True Set the state condition achievement conditions (True, False).
I1	X	\uparrow	0.00A	\swarrow	
P1	X	—	0W	\swarrow	
U2	X	—	0.0V	\swarrow	
I2	X	—	0.00A	\swarrow	
P2	X	—	0W	\swarrow	
AUX5	X	—	0.0V	\swarrow	
AUX6	X	—	0.0V	\swarrow	

Condition A is being met → Trigger
↑
Edge detection

3.11 Triggering on an OR or AND Trigger (Enhanced)

This section explains the following settings for triggering on an OR or AND trigger.

- Trigger source
- Edge detection condition (OR trigger)
- Achievement condition (AND trigger)
- Trigger condition

► **Features Guide: “OR Trigger (Enhanced)” and “AND Trigger (Enhanced)”**

ENHANCED OR Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

SIMPLE/ENHANCED

Setting
Simple Enhanced — **Set Setting to Enhanced.**

Type
OR — **Set Type to OR.**

Set Pattern — **Set the state and trigger conditions.**

Hold Off
0.00us — **Set the trigger hold off. ► section 3.3**

Setting the State and Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

Set the edge detection condition (\uparrow , \downarrow , IN, OUT, —).

Set the trigger level (set to the center value of the level width if the edge detection condition is set to IN or OUT).

Set the level width (when the edge detection condition is set to IN or OUT).

Set the hysteresis (∇ , ∇ , ∇).

	Edge	Level	Width	Hys
U1	\uparrow	0.0V	4.0V	∇
I1	—	0.00A	0.20A	∇
P1	—	0W	40W	∇
U2	—	0.0V	4.0V	∇
I2	—	0.00A	0.20A	∇
P2	—	0W	40W	∇
AUX5	—	0.0V	5.0V	∇
AUX6	—	0.0V	5.0V	∇
Ext	—			

ENHANCED AND Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

SIMPLE/ENHANCED

Setting

Simple **Enhanced**

Type

AND

Set Pattern

Hold Off

0.00 μ s

Set Setting to Enhanced.

Set Type to AND.

Set the state and trigger conditions.

Set the trigger hold off. ▶ section 3.3

Setting the State and Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

Set the achievement condition (H, L, IN, OUT, —).

Set the trigger level (set to the center value of the level width if the achievement condition is set to IN or OUT).

Set the level width (when the achievement condition is set to IN or OUT).

Set the hysteresis (∇ , ∇ , ∇).

	Condition	Level	Width	Hys
U1	—	0.0V	4.0V	∇
I1	—	0.00A	0.20A	∇
P1	—	0W	40W	∇
U2	—	0.0V	4.0V	∇
I2	—	0.00A	0.20A	∇
P2	—	0W	40W	∇
AUX5	—	0.0V	5.0V	∇
AUX6	—	0.0V	5.0V	∇

3.12 Triggering on a Period Trigger (Enhanced)

This section explains the following settings for triggering on a period trigger.

- Trigger source
- State condition
- Determination mode
- Reference time
- Trigger condition

► [Features Guide: “Period Trigger \(Enhanced\)”](#)

ENHANCED Period Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

SIMPLE/ENHANCED

Setting
Simple **Enhanced** — **Set Setting to Enhanced.**

Type
Period — **Set Type to Period.**

Set Pattern — **Set the state and trigger conditions.**

Hold Off
0.00us — **Set the trigger hold off. ► section 3.3**

Setting the State and Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

Set the state condition (H, L, or X (do not use as a trigger source)).

Set the trigger level.

	B State	Level	Hys
U1	H	0.0V	HL
I1	X	0.00A	HL
P1	X	0W	HL
U2	X	0.0V	HL
I2	X	0.00A	HL
P2	X	0W	HL
AUX5	X	0.0V	HL
AUX6	X	0.0V	HL

Set the hysteresis (~~HL~~, ~~HL~~, ~~HL~~).

Mode
T1 < T < T2 — **Set the determination mode.**

T1
0.02us

T2
0.03us

Set the reference time.*

Met
B → Reference time T → Met → B → Trigger

* Set T1 and T2 when the determination mode is T1 < T < T2 or T < T1, T2 < T.
Set Time when the determination mode is T < Time or T > Time.

3.12 Triggering on a Period Trigger (Enhanced)

Setting the Reference Mode (Mode)

Set what kind of relationship must be established between period T and the specified reference times (Time or T1 and T2) for the PX8000 to trigger.

T < Time	Period T must be shorter than the reference time (Time).
T > Time	Period T must be longer than the reference time (Time).
T1 < T < T2	Period T must be longer than reference time T1 and shorter than reference time T2.
T < T1, T2 < T	Period T must be shorter than reference time T1 or longer than reference time T2.

3.13 Triggering on a Pulse Width Trigger (Enhanced)

This section explains the following settings for triggering on a pulse width trigger.

- Trigger source
- State condition
- Determination mode
- Reference time
- Trigger condition

► [Features Guide: “Pulse Width Trigger \(Enhanced\)”](#)

ENHANCED Pulse Width Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

SIMPLE/ENHANCED

Setting
Simple Enhanced

Type
Pulse Width

Set Pattern

Hold Off
0.00us

Set Setting to Enhanced.

Set the trigger type to Pulse Width.

Set the state and trigger conditions.

Set the trigger hold off. ► section 3.3

Setting the State and Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

Set the state condition (H, L, or X (do not use as a trigger source)).

Set the trigger level.

	B State	Level	Hys
U1	H	0.0V	✓
I1	X	0.00A	✓
P1	X	0W	✓
U2	X	0.0V	✓
I2	X	0.00A	✓
P2	X	0W	✓
AUX5	X	0.0V	✓
AUX6	X	0.0V	✓

Pulse Width

Mode
B Between

T1
0.01us

T2
0.02us

Set the hysteresis (~~✓~~, ~~✓~~, ~~✓~~).

Set the determination mode.

Set the reference time.*

Achievement time
B → Trigger

* Set T1 and T2 when the determination mode is B Between.
Set Time when the determination mode is B < Time, B > Time, or B TimeOut.

3.13 Triggering on a Pulse Width Trigger (Enhanced)

Setting the Reference Mode (Mode)

Set what kind of relationship must be established between the state condition B achievement time and the specified reference times (Time or T1 and T2) for the PX8000 to trigger.

B < Time	The PX8000 triggers when the achievement time is shorter than the reference time (Time), and the state condition changes from being met to not being met.
B > Time	The PX8000 triggers when the achievement time is longer than the reference time (Time), and the state condition changes from being met to not being met.
B TimeOut	The PX8000 triggers when the achievement time is longer than the reference time (Time).
B Between	The PX8000 triggers when the achievement time is longer than reference time T1 and shorter than reference time T2, and the state condition changes from being met to not being met.

3.14 Triggering on a Wave Window Trigger (Enhanced)

This section explains the following settings for triggering on a wave window trigger.

- Source channel
Tolerance width, cycle frequency, and reference cycle
- Synchronization channel
- Trigger condition

► [Features Guide: “Wave Window Trigger \(Enhanced\)”](#)

ENHANCED Wave Window Trigger Menu

Press **SIMPLE/ENHANCED** and then the **Setting** soft key to select Enhanced. The following menu appears.

The screenshot shows a vertical menu with the following options and annotations:

- SIMPLE/ENHANCED** (header)
- Setting** (header)
- Simple** and **Enhanced** (radio buttons). Annotation: **Set Setting to Enhanced.**
- Type** (header)
- Wave Window** (radio button). Annotation: **Set Type to Wave Window.**
- Set Pattern** (header). Annotation: **Set the trigger conditions.**
- Hold Off** (header)
- 0.00us** (value). Annotation: **Set the trigger hold off. ► section 3.3**

Setting the Trigger Conditions (Set Pattern)

Press the **Set Pattern** soft key to display the following menu.

The screenshot shows the **Set Pattern** menu with the following sections and annotations:

- Wave Window** (header)
- Condition** and **Width** (headers for the table below)
- Table:**

	Condition	Width
U1	OFF	0.2V
I1	OFF	0.01A
P1	OFF	0.5W
U2	OFF	0.2V
I2	OFF	0.01A
P2	OFF	0.5W
AUX5	OFF	0.5V
AUX6	OFF	0.5V

- Cycle Frequency** (header)
- 50Hz** (value). Annotation: **Set the cycle frequency.**
- Reference Cycle** (header)
- 1** (value). Annotation: **Set the reference cycle.**
- Sync. Ch** (header)
- U1** (value). Annotation: **Set the synchronization channel (Auto, U1-U4, I1-I4, P1-P4, AUX3-AUX8).**
- Level** (header)
- 0.0V** (value)
- Hysteresis** (header)
- ≠** (value). Annotation: **Set the level for detecting the start and end points, and set the detection hysteresis.***

* Set when the synchronization channel is U1 to U4, I1 to I4, P1 to P4, or AUX3 to AUX8.

3.15 Triggering the PX8000 Manually (Manual Trigger)

This section explains how to trigger the PX8000 manually.

► [Features Guide: “Trigger Types \(Type\)”](#)

Press **MANUAL TRIG**.

4.1 Setting Conditions for Waveform Acquisition

This section explains the following settings for acquiring waveforms.

- Record length
- Acquisition mode
- Number of waveforms to acquire and attenuation constant
- Time base
- Executing logger setup

► [Features Guide: “Waveform Acquisition”](#)

ACQUIRE Menu

Press **ACQUIRE** to display the following menu.

When the Acquisition Mode Is Set to Normal or Envelope

ACQUIRE	
Record Length 1M	Set the record length.
Acquisition Mode Normal	Set the acquisition mode to Normal or Envelope.
Trigger Mode Auto	Set the trigger mode. ► section 3.1
Acquisition Count Infinite	Set the number of waveform acquisitions.
Time Base Int Ext	Set the time base (Int, Ext).
Execute Logger Setup	Execute Logger Setup.*

Time Base Int Ext	Set the pulse/rotation.
Pulse/Rotate ii	
Execute	

* A confirmation message will appear.

When the Acquisition Mode Is Set to Average

ACQUIRE	
Record Length 1M	Set the record length.
Acquisition Mode Average	Set the acquisition mode to Average.
Trigger Mode Auto	Set the trigger mode. ► section 3.1
Acquisition Count Infinite	Set the number of waveform acquisitions.
Weight 16	Set the attenuation constant.
Time Base Int Ext	Set the time base (Int, Ext).
Execute Logger Setup	Execute Logger Setup.*

Time Base Int Ext	Set the pulse/rotation.
Pulse/Rotate ii	
Execute	

* A confirmation message will appear.

Setting the Acquisition Mode (Acquisition Mode)

- Normal: Displays waveforms without processing the sampled data. You can set the number of waveforms to acquire with the jog shuttle.
- Envelope: Displays waveforms in envelope mode. You can set the number of waveforms to acquire with the jog shuttle.
- Average: Displays averaged waveforms. You can set the attenuation constant and the number of times to average with the jog shuttle.

4.2 Starting and Stopping Waveform Acquisition

This section explains how to start and stop waveform acquisition.

► [Features Guide: “Waveform Acquisition \(START/STOP\)”](#)

Waveform Acquisition (START/STOP)

Press **START/STOP** to start or stop waveform acquisition.

When the START/STOP key is illuminated, the PX8000 is acquiring waveforms.

Note

If every numeric data (see chapter 6) is displayed as no data (-----) even when you start waveform acquisition, check the following items.

- Is the numeric measurement setting set to ON? ► [section 7.1](#)
 - Is the trigger set properly?
 - Trigger mode ► [section 3.1](#)
 - Trigger position and trigger delay ► [section 3.2](#)
 - Trigger hold off ► [section 3.3](#)
 - Trigger conditions according to trigger type ► [sections 3.4 to 3.15](#)
-

5.1 Selecting the Display Mode



This section explains how to set the type of display to show.

- Display mode

► [Features Guide: “Display Mode and Display Settings”](#)

DISPLAY MODE menu

Press **DISPLAY MODE** to display the following menu.

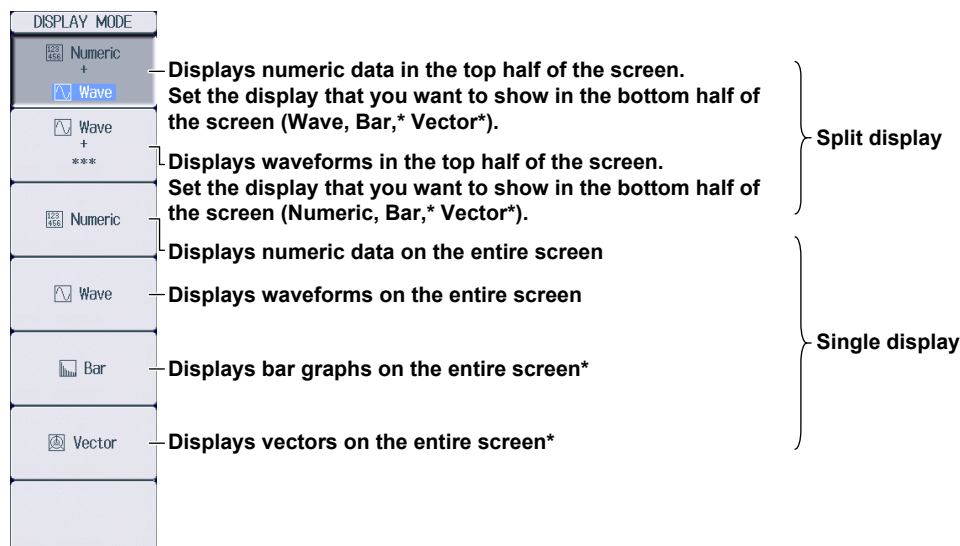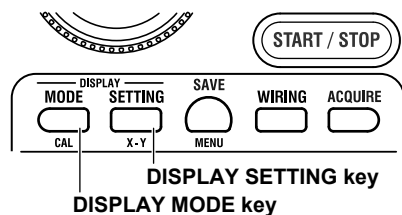

* These settings are available on models with the harmonic measurement (/G5) option.

DISPLAY SETTING Menu

Press **DISPLAY SETTING**. The SETTING menu of the display you specified on the DISPLAY MODE menu appears.

If you specified a split display in which the half of the screen is set to Numeric or Wave on the DISPLAY MODE menu, the SETTING menu for the top half of the screen and that of the bottom half of the screen toggles each time you press DISPLAY SETTING.

For details on the different SETTING menus, see the following sections.

NUMERIC SETTING menu ► [section 6.1](#)

WAVE SETTING menu ► [section 8.1](#)

BAR SETTING menu ► [section 9.1](#)

VECTOR SETTING menu ► [section 10.1](#)


6.1 Switching the Displayed Page

This section explains how to switch the displayed numeric data page.

► [Features Guide: “Numeric Data Display Settings”](#)
[“Switching the Displayed Page”](#)

NUMERIC SETTING menu

1. Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the NUMERIC SETTING menu.

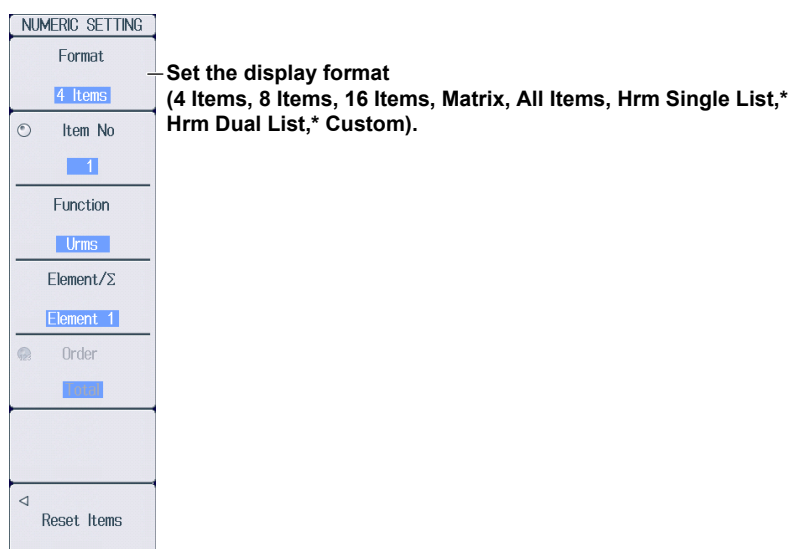

* These settings are available on models with the harmonic measurement (/G5) option.

2. Set the display format, and then press **ESC** to clear the menu.

Note


If every numeric data is displayed as no data (-----), check the following items.

- Is waveform acquisition running? ► section 4.2
- Is the numeric measurement setting set to ON? ► section 7.1
- Is the trigger set properly?
 - Trigger mode ► section 3.1
 - Trigger position and trigger delay ► section 3.2
 - Trigger hold off ► section 3.3
 - Trigger conditions according to trigger type ► sections 3.4 to 3.15

When the Display Format Is 4 Items, 8 Items, 16 Items, Matrix, All Items, or Custom

Press the up and down **arrow** keys (▲, ▼) to switch the page.


- You can switch the displayed page separately for the 4 Items, 8 Items, 16 Items, Matrix, All Items, and Custom displays.
 - If the display format is set to All Items in single display mode (see section 5.1), the top half of the display of page 1 is constantly displayed, and the bottom half of the display changes for subsequent pages. In split display mode (see section 5.1), the entire numeric data displayed in the top or bottom half of the screen switches.
- In addition, if the display format is set to All Items, you can switch pages using soft keys without clearing the menu as explained in step 2 on the previous page.
- For the Custom display, you can switch between pages when the display is set so that the total number of displayed items is more than the number of items that can be displayed on one page (see section 6.6).

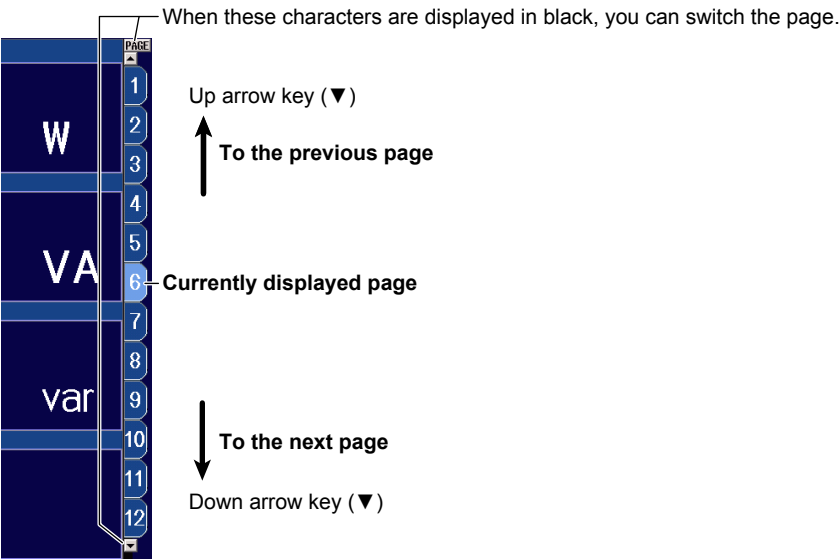

When the Display Format Is Hrm Single List or Hrm Dual List (/G5 Option)

1. Press the left and right **arrow** keys (◀, ▶) to select either the measurement function side (the left side of the screen) or the harmonic order data side (the right side of the screen).
2. Press the up and down **arrow** keys (▲, ▼) to switch the page.

Use the left and right arrow keys (◀, ▶) to switch between the measurement function side and harmonic data side.

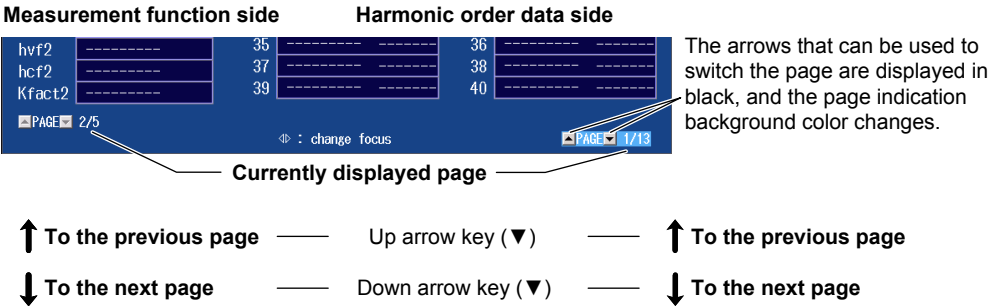

6.2 Changing the Displayed Items on the 4-, 8-, and 16-Value Displays

This section explains the following settings for the displayed items on the 4-, 8-, and 16-value displays.

- Item number
- Measurement function
- Element and wiring unit
- Order (harmonic order, /G5 option)
- Resetting the displayed items

► **Features Guide: “4-, 8-, and 16-Value Displays (4 Items/8 Items/16 Items).”**

NUMERIC SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the NUMERIC SETTING menu.

NUMERIC SETTING							
Format 4 Items	Set the display format to 4 Items, 8 Items, or 16 Items.						
Item No 1	Select the item number that you want to set. <table border="0"><tr><td>(For 4 Items: 1-48</td><td>)</td></tr><tr><td>(For 8 Items: 1-96</td><td>)</td></tr><tr><td>(For 16 Items: 1-192</td><td>)</td></tr></table>	(For 4 Items: 1-48)	(For 8 Items: 1-96)	(For 16 Items: 1-192)
(For 4 Items: 1-48)						
(For 8 Items: 1-96)						
(For 16 Items: 1-192)						
Function Urms	Set the measurement function (None, other functions—for details on the various measurement functions, see “Items That This Instrument Can Measure” in the Features Guide).						
Element/ Σ Element 1	Set the element and wiring unit (Element 1-Element 4, ΣA , ΣB).						
Order Total	Set the harmonic order (Total, 0-500).* You can set this setting only when you have selected a measurement function that includes a harmonic order.						
Reset Items	Set the resetting of displayed items.						

* These settings are available on models with the harmonic measurement (/G5) option.

Example of the 4 Items Display

Urms1	0.00	V
Irms1	0.0000	A
P1	0.00	W
Umn1	0.00	V

Note

If every numeric data is displayed as no data (-----), check the referenced sections under “Note” in section 6.1.

Resetting the Displayed Items (Reset Items)

Press the **Reset Items** soft key to display the following menu.

NUMERIC SETTING

Format

4 Items

Item No

1

Function

Urms

Element/ Σ

Reset Items

Reset Items Exec

Clear Current Page

Clear All Pages

Resets the arrangement of the displayed items on all pages

The arrangement pattern varies depending on the number of installed elements.

Sets all displayed measurement functions to None*

Sets all measurement functions on all pages to None*

* The measurement functions displayed on the screen are cleared, and every numeric data is displayed as no data.

Switching the Page

To set items on pages that are not currently shown, switch to these pages. For details on how to switch pages, see section 6.1.

6.3 Changing the Displayed Items on the Matrix Display

This section explains the following settings for the displayed items on the Matrix display.

- Item number
- Measurement function
- Order (harmonic order, /G5 option)
- Display column
 - Number of columns, element and wiring unit
- Resetting the displayed items

► [Features Guide: “Matrix Display \(Matrix\)”](#)

NUMERIC SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the NUMERIC SETTING menu.

NUMERIC SETTING	
Format Matrix	Set the display format to Matrix.
Item No 1	Select the item number that you want to set (1-81).
Function Urms	Set the measurement function (None, other functions—for details on the various measurement functions, see “Items That This Instrument Can Measure” in the Features Guide).
Order Total	Set the harmonic order (Total, 0-500).* You can set this setting only when you have selected a measurement function that includes a harmonic order.
Column Settings	Configure the columns to display.
Reset Items	Set the resetting of displayed items.

* These settings are available on models with the harmonic measurement (/G5) option.

Matrix Display Example

		Element 1	Element 2	Σ A(3P3W)	-----	-----	-----
Urms	[V]	0.00	0.00	0.00			
Irms	[A]	0.084m	0.159m	0.122m			
P	[W]	-0.0000	-0.0000	-0.0000			
S	[VA]	0.0000	0.0000	0.0000			
Q	[var]	0.0000	0.0000	0.0000			
λ	[]	Error	Error	Error			
φ	[°]	Error	Error	Error			
Umn	[V]	0.00	0.00	0.00			
Iac	[A]	0.083m	0.103m	0.093m			

Note

If every numeric data is displayed as no data (-----), check the referenced sections under “Note” in section 6.1.

6.3 Changing the Displayed Items on the Matrix Display

Setting the Columns to Display (Column Settings)

Press the **Column Settings** soft key to display the following menu.

Column Settings

Columns

4 6

Column No

||

Element/Σ

Element 1

Reset Columns

Set the number of columns (4, 6).

Set the column number (1-6).

Set the element and wiring unit (None, Element 1-Element 4, ΣA, ΣB).

Resets the element and wiring unit settings of each column

Resetting the Displayed Items (Reset Items)

Press the **Reset Items** soft key to display the following menu.

NUMERIC SETTING

Format

Matrix

Item No

1

Function

Urms

Reset Items

Reset Items Exec

Clear Current Page

Clear All Pages

Resets the arrangement of the displayed items on all pages
The arrangement pattern varies depending on the number of installed elements.

Sets all displayed measurement functions to None*

Sets all measurement functions on all pages to None*

* The measurement functions displayed on the screen are cleared, and every numeric data is displayed as no data.

Switching the Page

To set items on pages that are not currently shown, switch to these pages. For details on how to switch pages, see section 6.1.

6.4 Changing the All Items Display


This section explains the following All Items display settings.

- Order (harmonic order, /G5 option)
- Switching the Page

► Features Guide: “All Items Display (All Items)”

NUMERIC SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the NUMERIC SETTING menu.

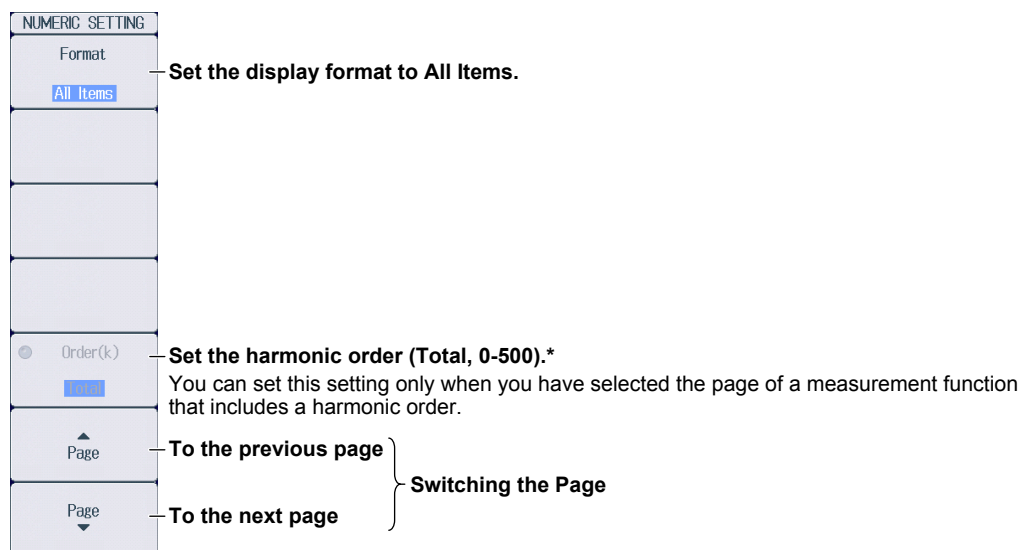

All Items Display example

	Element 1	Element 2	Σ A(3P3W)
Voltage	100V	100V	
Current	10mA	10mA	
Urms [V]	0.00	0.00	0.00
Irms [A]	0.084m	0.165m	0.125m
P [W]	-0.0000	-0.0000	-0.0000
S [VA]	0.0000	0.0000	0.0000
Q [var]	0.0000	0.0000	0.0000
λ []	Error	Error	Error
φ [°]	Error	Error	Error
fU [Hz]	Error	Error	
fI [Hz]	Error	Error	

Note

- On the All Items display, you cannot select individual display items and change their measurement function, element, or wiring unit. If you switch to the Matrix display, you can change the measurement functions, elements, and wiring units using the displayed table (see section 6.3).
- If every numeric data is displayed as no data (-----), check the referenced sections under “Note” in section 6.1.

6.5 Changing the Harmonics List Display (Option)

This section explains the following settings for the harmonics list display (Hrm List). These settings are available on models with the harmonic measurement (/G5) option.

- List number
- Measurement function
- Element and wiring unit

► **Features Guide: “Single Harmonics and Dual Harmonics Lists (Hrm Single List/Hrm Dual List; option)”**

NUMERIC SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the NUMERIC SETTING menu.

The screenshot shows the NUMERIC SETTING menu with the following options and annotations:

- Format:** Hrm Single List. **Set the display format to Hrm Single List or Hrm Dual List.**
- Item No:** 1. **Select the list number that you want to set (1, 2).** Function, element, and wiring unit settings that you make for list number 2 are also reflected in the right column of the harmonic order data of the dual harmonics list.
- Function:** U. **Set the measurement function (U, I, P, S, Q, λ , Φ , ΦU , ΦI , Z, Rs, Xs, Rp, Xp).**
- Element/ Σ :** Element 1. **Set the element and wiring unit (Element 1-Element 4, ΣA , ΣB).**

Hrm Single List Display Example

Measurement function side			Harmonic order data side		
fPLL:U1	60.001 Hz		Order	U1 [V]	hdf[%]
Urms1	3.956 V		Total	3.545	
Irms1	349.58 A		1	2.706	76.316
P1	0.7715 kW		3	0.670	18.893
S1	1.3831 kVA		5	0.644	18.173
Q1	1.1479 kvar		7	0.169	4.760
$\lambda 1$	0.5578		9	0.392	11.048
$\Phi 1$	G56.10 °		11	0.025	0.702
			13	0.277	7.807
			15	0.043	1.219
			17	0.202	5.703
			19	0.080	2.268
			Order	U1 [V]	hdf[%]
			dc	1.786	50.377
			2	0.229	6.472
			4	0.556	15.676
			6	0.222	6.256
			8	0.288	8.121
			10	0.210	5.913
			12	0.160	4.504
			14	0.193	5.443
			16	0.080	2.258
			18	0.173	4.875

Note

If every numeric data is displayed as no data (-----), check the referenced sections under “Note” in section 6.1.

Hrm Dual List Display Example

Measurement function side			Harmonic order data side					
fPLL:U1	60.001 Hz	Order	U1 [V]	hdf [%]	Order	I1 [A]	hdf [%]	
		Total	3.545		Total	348.77		
		dc	-----		dc	-----		
		1	2.706	76.316	1	314.64	90.212	
		2	1.786	50.377	2	0.01	0.004	
		3	0.670	18.893	3	104.88	30.070	
		4	0.229	6.472	4	0.01	0.002	
		5	0.644	18.173	5	62.92	18.039	
		6	0.556	15.676	6	0.01	0.003	
		7	0.169	4.760	7	44.93	12.883	
		8	0.222	6.256	8	0.01	0.002	
		9	0.392	11.048	9	34.95	10.021	
		10	0.288	8.121	10	0.01	0.002	
Urms1	3.956 V							
Irms1	349.58 A							
P1	0.7715 kW							
S1	1.3831 kVA							
Q1	1.1479 kvar							
λ1	0.5578							
φ1	656.10 °							
PAGE 1/14			⏏ : change focus			PAGE 1/50		

Note

On the harmonics list displays, you can change the measurement function, element, and wiring unit for the selected list, but you cannot change these settings for each individual display item.

Switching the Page

You can switch the page to display other items. For details on how to switch pages, see section 6.1.

6.6 Setting the Custom Display

This section explains the following Custom display settings.


- Loading display configuration files
- Loading background files
- Display configuration

Total items, items per page, custom items (item number, measurement function, element and wiring unit, harmonic order, display position, font size, font color), saving custom display configuration files

► [Features Guide: “Custom Display \(Custom\)”](#)

NUMERIC SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the NUMERIC SETTING menu.

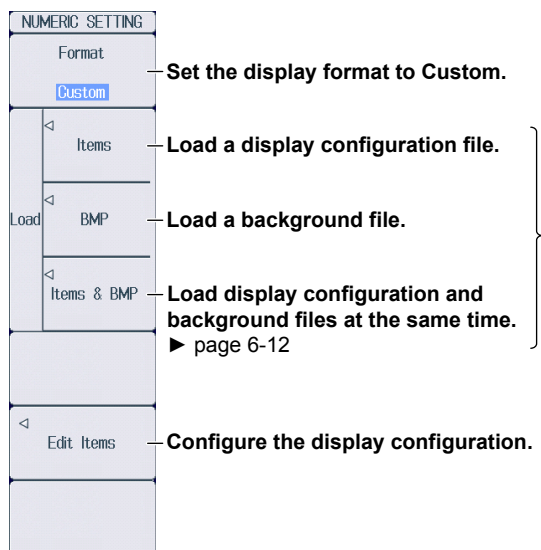

The screenshot shows the NUMERIC SETTING menu with the following options and annotations:


- Format**: Set the display format to Custom.
- Load**: Load a display configuration file.
- Items**: Load a background file.
- BMP**: Load display configuration and background files at the same time. (page 6-12)
- Items & BMP**: Load display configuration and background files at the same time. (page 6-12)
- Edit Items**: Configure the display configuration.

You can load files for the custom display.
Display configuration files: TXT format
Background file: BMP format

- You can use the “Edit Items” menu described below to change the display configuration that you have loaded.
- To load both a display configuration file and background file at the same time, load the display configuration file.

Setting the Display Configuration (Edit Items)

1. Press the **Edit Items** soft key to display the following menu.

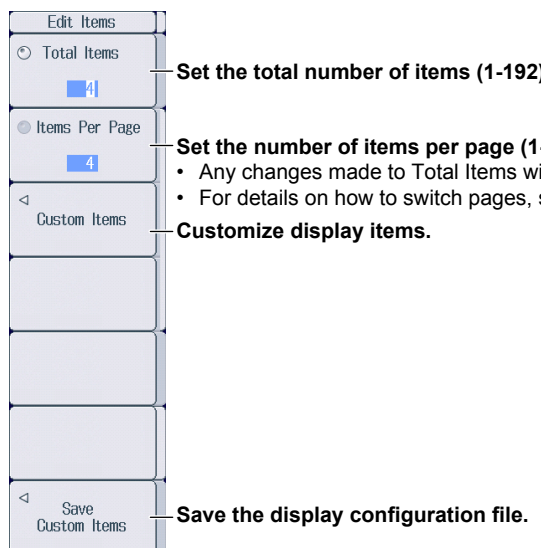

The screenshot shows the Edit Items menu with the following options and annotations:

- Total Items**: Set the total number of items (1-192).
- Items Per Page**: Set the number of items per page (1-192).
 - Any changes made to Total Items will change the Items Per Page setting, and vice-versa.
 - For details on how to switch pages, see section 6.1.
- Custom Items**: Customize display items.
- Save Custom Items**: Save the display configuration file.

Customizing Display Items (Custom Items)

- Press the **Custom Items** soft key to display the following screen.

(X, Y)

Element 1

Voltage rms **Current rms** **Power**

0.0164 **0.083 m** **0.000 m**

mean 0.0000 mean 0.000 m VA 0.001 m
 dc 0.0009 dc 0.013 m var -0.001 m
 r-mn 0.0000 r-mn 0.000 m PF 0.0119
 ac 0.0164 ac 0.082 m deg D89.32
 max 0.0621 max 0.400 m max 0.015 m
 min -0.0579 min -0.375 m min -0.013 m
 CF 3.785 CF 4.791

Voltage frequency **Error** Current frequency **Error**

Custom Items

Item No 2

Function Urms

Element/Σ Element 1

Order

X Pos 20

Y Pos 100

Font Size 48

Font Color Yellow

Select the item number that you want to set (1-the Total Items setting).

Set the measurement function (None, other functions—for details on the various measurement functions, see “Items That This Instrument Can Measure” in the Features Guide).

Set the element and wiring unit (Element 1-Element 4, ΣA, ΣB).

When Function is set to None:
Set the character string (up to 15 characters).

When the measurement function includes a harmonic order:
Set the harmonic order (Total, 0-500; G5 option).

Set the display position.

- X Pos: 0 (left edge of the screen)-800 (right edge of the screen)
- Y Pos: 0 (top of the screen)-671 (bottom of the screen)

Set the font size (14, 16, 20, 24, 32, 48, 64, 96, 128).

Set the font color (Yellow, Green, Magenta, Cyan, Red, Orange, Light Blue, Purple, Blue, Pink, Light Green, Dark Blue, Blue Green, Salmon Pink, Mid Green, Gray, White, Dark Gray, Blue Gray, Black).

Note

If every numeric data is displayed as no data (-----), check the referenced sections under “Note” in section 6.1.

Saving Display Configuration Files (Save Custom Items)

- Press the **Save Custom Items** soft key to display the following menu.

Save Custom Items

File List Set the save destination. ► section 22.3


File Name Set the file name. ► section 22.3

Execute Save Starts saving

Note that if a file with the same name exists in the destination folder, it will be overwritten without warning.
File names are not case-sensitive.

Loading Display Configuration and Background Files at the Same Time (Load Items & Bmp)

On the NUMERIC SETTING menu on page 6-10, click the **Items & Bmp** soft key to display the following screen.

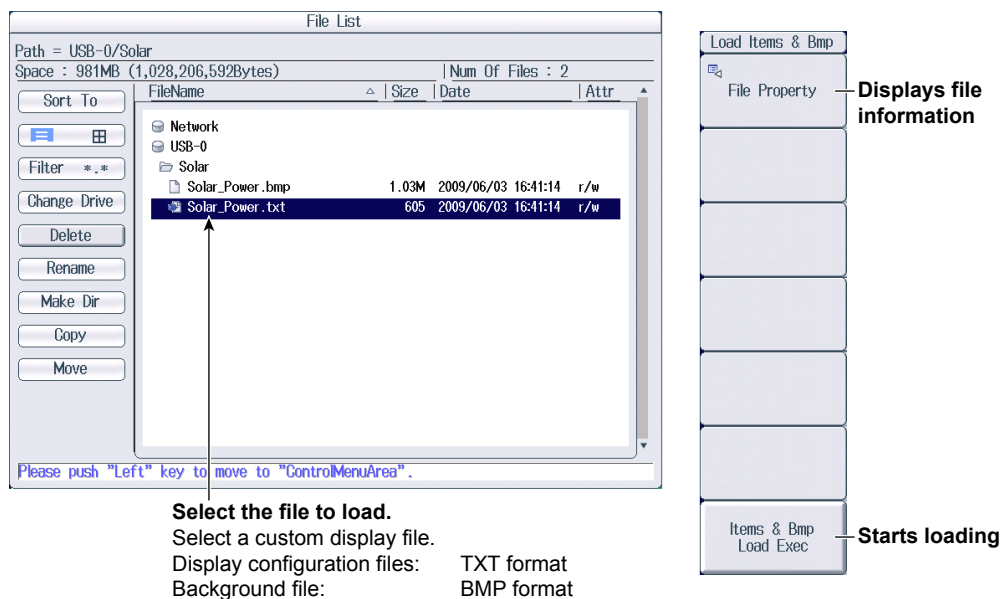


To load both a display configuration file and background file at the same time, load the display configuration file.

However, an error will occur if a background file that has the same name as the display configuration file is not present in the save destination folder of the display configuration file.

For the operating procedure, see section 22.10.

Example of Loading a File for the Custom Display

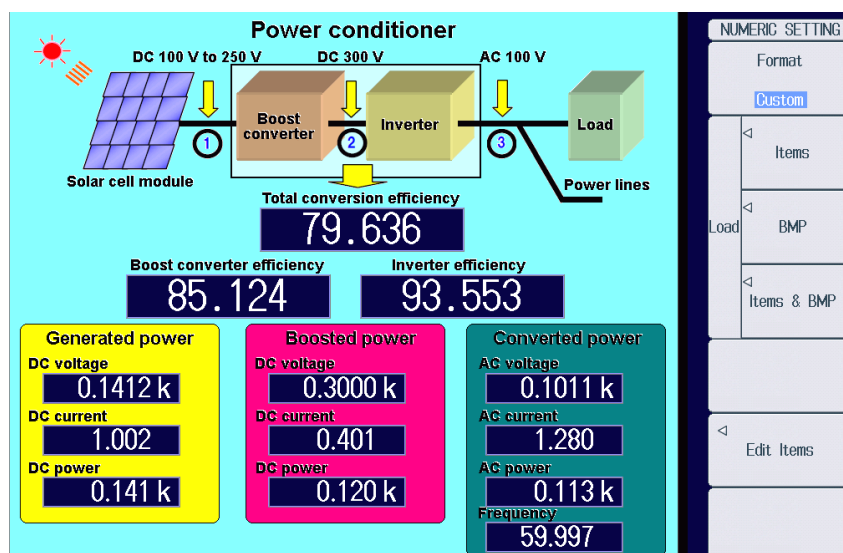

Note

After you properly load a display configuration file and a background file, if you restart the PX8000 and the same background file is not in the same location, the background will return to its default.

Switching the Page

You can switch between pages when the display is set so that the total number of displayed items is more than the number of items that can be displayed on one page. For details on how to switch pages, see section 6.1.


7.1 Turning Numeric Measurement On and Off

This section explains how to turn numeric measurement on and off.

► [Features Guide: “Turning Numeric Measurement On and Off \(Numeric Measure\)”](#)

NUMERIC Menu

Press **NUMERIC** to display the following menu.

NUMERIC
Numeric Measure
OFF ON
Period
Zero Cross
◀ Harmonics
 Next 1/2

Turns numeric measurement on and off

To measure voltage, current, power, and other measurement functions, set this to ON. If this is set to OFF, none of the measurement functions will be measured, and every numeric data will be displayed as no data (-----).

Note

If every numeric data (see chapter 6) is displayed as no data (-----) even when you turn numeric measurement on, check the following items.

- Is waveform acquisition running? ► [section 4.2](#)
- Is the trigger set properly?
 - Trigger mode ► [section 3.1](#)
 - Trigger position and trigger delay ► [section 3.2](#)
 - Trigger hold off ► [section 3.3](#)
 - Trigger conditions according to trigger type ► [sections 3.4 to 3.15](#)

7.2 Setting the Calculation Period


This section explains the following settings for measuring and computing measurement functions of normal measurement.

- Calculation period
- External signal status
- Cursor start and end points
- Search zero cross

► Features Guide: “Calculation Period (Period)”

NUMERIC Menu


Press **NUMERIC** to display the following menu.


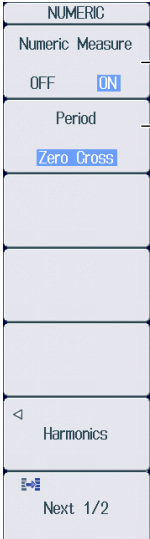


Set Numeric Measure to ON.


Calculation period (Zero Cross, Ext Gate, Cursor)

When the calculation period is Ext Gate



Set the external signal status ( , )

When the calculation period is Cursor




Set the cursor start and end points.

Set the search zero cross

Setting Search Zero Cross (Search Zero Cross)

Press the **Search Zero Cross** soft key to display the following menu.

When Start Position is selected for the cursor start and end point setting



Set the cursor start and end points.


Set the zero-crossing search source.

Set the edge.

Moves to the nearest zero-crossing position after the Start Position

Moves to the nearest zero-crossing position before the Start Position


When End Position is selected for the cursor start and end point setting



Moves to the nearest zero-crossing position after the End Position

Moves to the nearest zero-crossing position before the End Position

When both Start Position and End Position are selected for the cursor start and end point setting



Moves to the nearest zero-crossing position after the Start Position while maintaining the cursor span

Moves to the nearest zero-crossing position before the Start Position while maintaining the cursor span

7.3 Setting Numeric Data Averaging

This section explains the following settings for exponential averaging (Exp) and moving averaging (Lin) of numeric data.

- Averaging type
- Attenuation constant
- Averaging count

► [Features Guide: “Averaging \(Averaging\)”](#)

NUMERIC Menu

1. Press **NUMERIC** to display the following menu.

NUMERIC	
Numeric Measure	Set Numeric Measure to ON.
OFF	ON
Period	
Zero Cross	
<	Harmonics
Next 1/2	Displays the second page of the menu

2. Press the **Next 1/2** soft key to display the 2/2 menu.

NUMERIC	
Averaging	Set the averaging type (OFF, Exp, Lin).
OFF	Exp
Count	
2	
<	User Defined Function
	Formula
	Phase
180 degrees	
Next 2/2	

When averaging type is Exp

Pattern	
1-2	FL
Averaging	
OFF	Exp
Count	
2	Set the attenuation constant (2-64).
<	User Defined

When averaging type is Lin

Pattern	
1-2	FL
Averaging	
OFF	Exp
Count	
8	Set the averaging count (8-64).
<	User Defined

7.4 Setting User-Defined Functions

This section explains the following settings for user-defined functions.

- Turning computation on and off
- Computation name
- Unit
- Equation

► [Features Guide: “User-Defined Functions \(User Defined Function\)”](#)

NUMERIC Menu

1. Press **NUMERIC** to display the following menu.

NUMERIC

Numeric Measure

OFF **ON** — Set Numeric Measure to ON.

Period

Zero Cross

Harmonics

Next 1/2 — Displays the second page of the menu

2. Press the **Next 1/2** soft key to display the 2/2 menu.

NUMERIC

Averaging

OFF **Exp** Lin

Count

2

User Defined Function — Set the user-defined function.

Formula

Phase

180 degrees

Next 2/2

Setting User-Defined Functions (User Defined Function)

Press the **User Defined Function** soft key to display the following screen.

Set the equation.

User Defined Function		Settings		
Function 1	<input type="checkbox"/> OFF <input checked="" type="checkbox"/> ON	Name	P-loss	Unit
Expression	P(E1)-P(E2)			
Function 2	<input type="checkbox"/> OFF <input checked="" type="checkbox"/> ON	Name	U-ripple	Unit
Expression	(UPPK(E1)-UMPK(E1))/2/UDC(E1)*100			
Function 3	<input type="checkbox"/> OFF <input checked="" type="checkbox"/> ON	Name	I-ripple	Unit
Expression	(IPPK(E1)-IMPK(E1))/2/IDC(E1)*100			
Function 4	<input type="checkbox"/> OFF <input checked="" type="checkbox"/> ON	Name	D-UrmsR	Unit
Expression	DELTAU1RMS(SA)			
Function 5	<input type="checkbox"/> OFF <input checked="" type="checkbox"/> ON	Name	D-UrmsS	Unit
Expression	DELTAU2RMS(SA)			
F01-F05		F06-F10		F11-F15

User Defined
 User Defined
F01-F05

Displays the setup screen for
user-defined functions F1 to F5

User Defined
 User Defined
F06-F10

Displays the setup screen for
user-defined functions F6 to F10

User Defined
 User Defined
F11-F15

Displays the setup screen for
user-defined functions F11 to F15

User Defined
 User Defined
F16-F20

Displays the setup screen for
user-defined functions F16 to F20

7.5 Setting Apparent Power, Reactive Power, and Corrected Power Equations


This section explains the following settings for the apparent power, reactive power, and corrected power equations.

- Apparent power equation
 - Apparent power and reactive power computation types
 - Corrected power equation
- Applicable standard and coefficients


► [Features Guide: “Apparent Power, Reactive Power, and Corrected Power Equations \(Formula\)”](#)

NUMERIC Menu

1. Press **NUMERIC** to display the following menu.

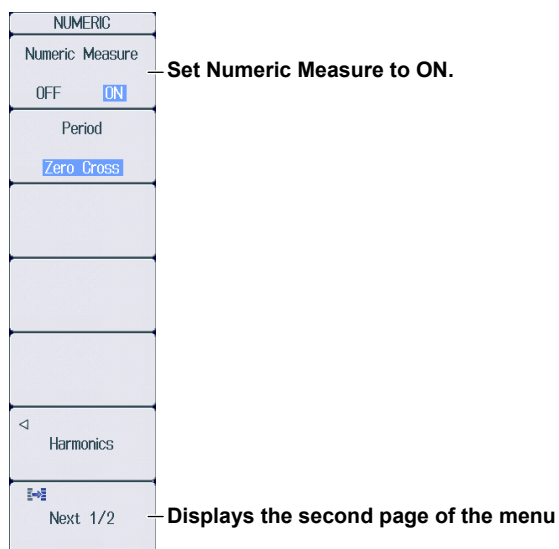

2. Press the **Next 1/2** soft key to display the 2/2 menu.

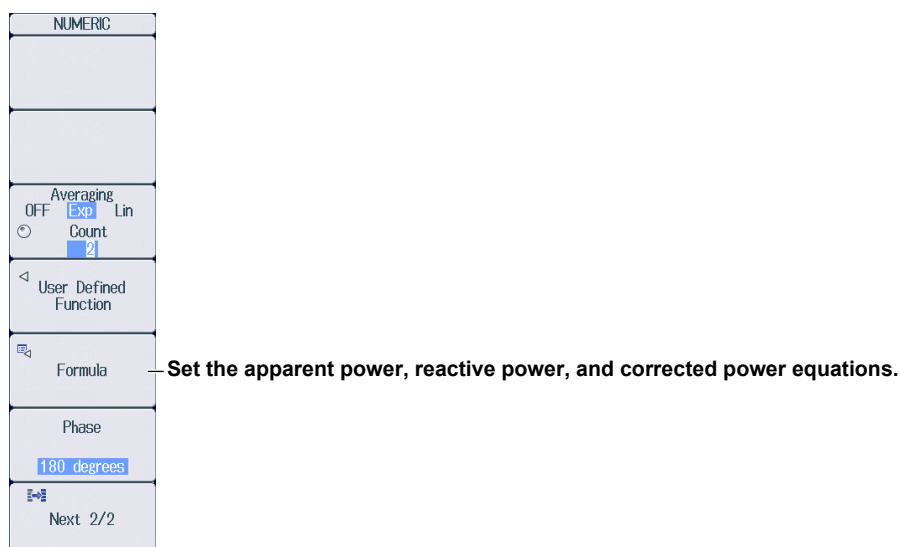

Setting Apparent Power, Reactive Power, and Corrected Power Equations (Formula)

Press the **Formula** soft key to display the following screen.

Set the apparent power equation
($U_{rms} \cdot I_{rms}$, $U_{mean} \cdot I_{mean}$, $U_{dc} \cdot I_{dc}$, $U_{mean} \cdot I_{rms}$, $U_{rmean} \cdot I_{rmean}$).

S Formula:

S,Q Formula: Type 2 Type 3

$P\Sigma = P1+P2+P3$

$S\Sigma = S1+S2+S3$

$Q\Sigma = Q1+Q2+Q3$ For 3P4W

Corrected power equation

Pc Formula:

Select standard:

P1 =

P2 =

Set the apparent power and reactive power computation types (Type 1, Type 2, Type 3†).

Set the applicable standard (IEC76-1(1976), IEC76-1(1993)).

Set the coefficients (0.0001-9.9999).
When Select standard is IEC76-1(1976), set coefficients P1 and P2.

† These settings are available on models with the harmonic measurement (/G5) option.


7.6 Setting the Phase Difference Display Format

This section explains how to set the phase difference display format.


► [Features Guide: “Phase Difference Display Format \(Phase\)”](#)

NUMERIC Menu

1. Press **NUMERIC** to display the following menu.

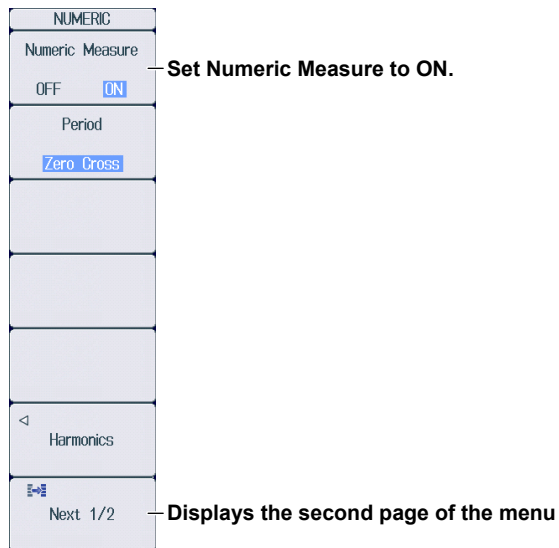

2. Press the **Next 1/2** soft key to display the 2/2 menu.

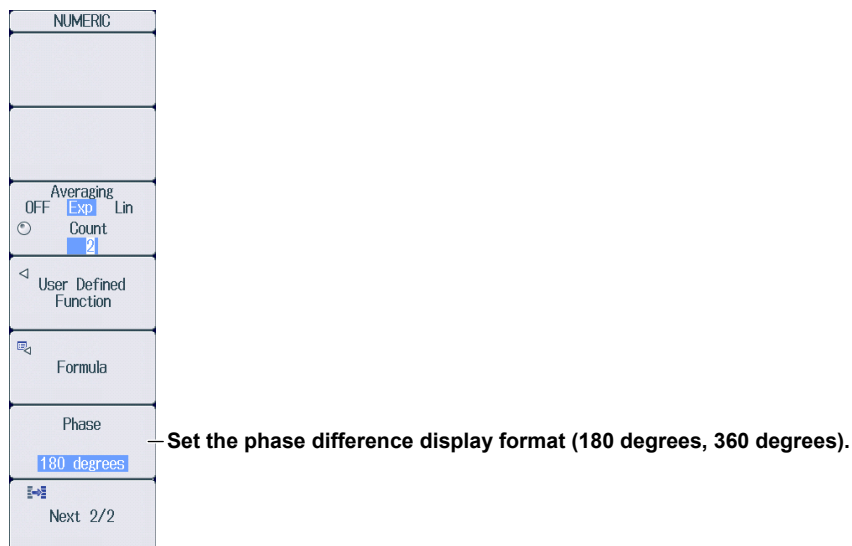

7.7 Setting Harmonic Measurement Conditions


This section explains the following settings for harmonic measurement conditions. These settings are available on models with the harmonic measurement (/G5) option.

- Turning harmonic measurement on and off
- PLL source
- Measured harmonic order
- Distortion factor equation
- Harmonic measurement start point

► [Features Guide: “Harmonic Measurement Conditions \(Harmonics; option\)”](#)


NUMERIC Menu

Press **NUMERIC** to display the following menu.

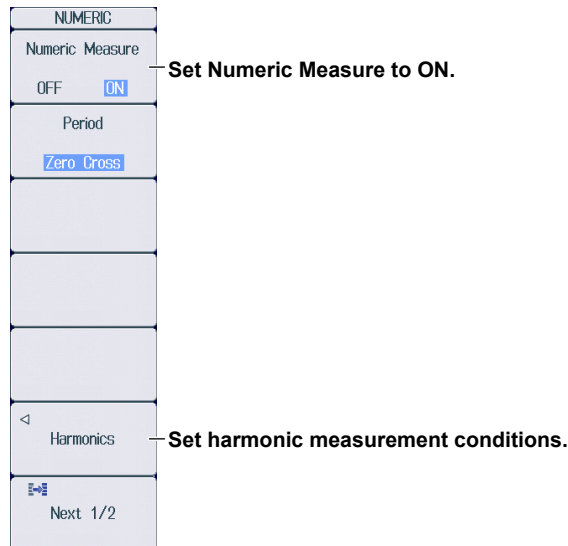

Harmonics Menu

Press the **Harmonics** soft key to display the following menu.

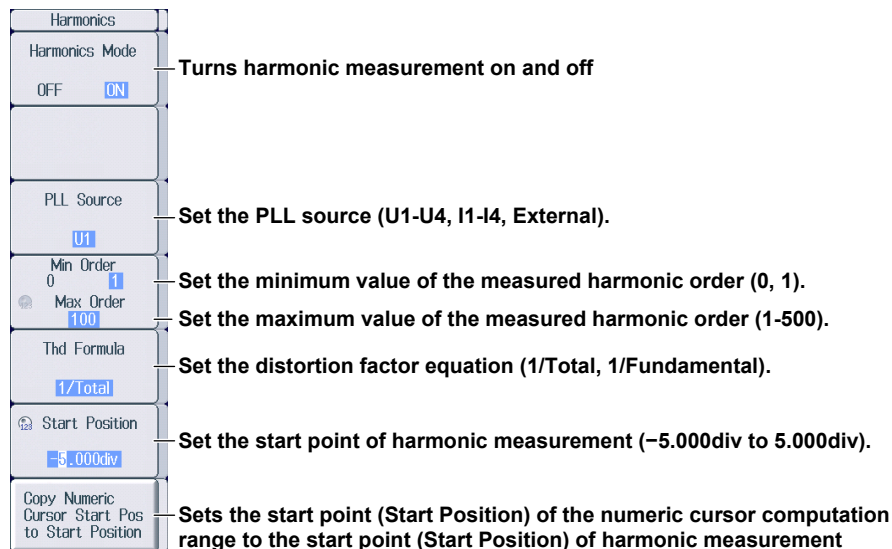

8.1 Setting the Waveform Display


This section explains the following settings for displaying waveforms.

- Waveform display format
- Detailed settings of the waveform display
Turning waveform display on and off, waveform color, waveform mapping, waveform label, vertical zoom
DIV: Offset value, waveform's vertical position, magnification
SPAN: Upper and lower limits of the display range
Horizontal (time scale) zoom ► chapter 12
- Interpolation method
- Grid
- Turning the display of scale values on and off
- Turning the trace label display on and off
- Extra window

► **Features Guide: “Waveform Display Settings”**

WAVE SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the WAVE SETTING menu.

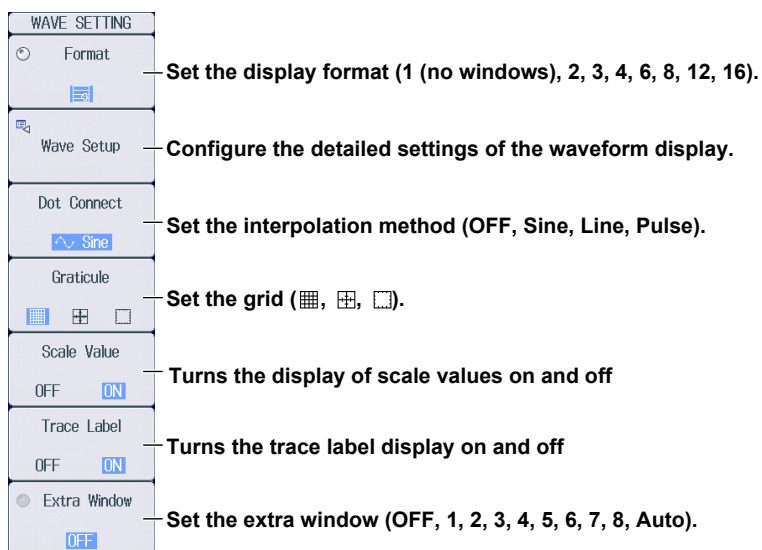

Configuring Detailed Settings of the Waveform Display (Wave Setup)

Press the **Wave Setup** soft key to display the following screen.

These settings are shared between the U menu, I menu, POWER menu, and AUX menu. ► **chapter 2**

Turns the waveform display on and off
Set this to turn all waveforms on and off.

Set the waveform label.
Set the vertical zoom.
For DIV: Set the offset value, waveform's vertical position, and magnification.
For SPAN: Set the upper and lower limits of the display range.

	Disp	Map	Label	V Scale	Offset	Position	V Zoom
All	ON	User					
CH1 (U1)	ON	1	U1	DIV	0.0V	0.00div	x 1
CH2 (I1)	ON	2	I1	SPAN	10000mA	-10000mA	
P1	ON	3	P1	DIV	0W	0.00div	x 2
CH3 (U2)	OFF	4	U2	DIV	0mV	0.00div	x 1
CH4 (I2)	OFF	5	I2	DIV	0mA	0.00div	x 1
P2	OFF	6	P2	DIV	0mW	0.00div	x 2
CH5 (AUX5)	ON	7	AUX5	DIV	0mV	0.00div	x 1
CH6 (AUX6)	OFF	8	AUX6	DIV	0.00E+03	0.00div	x 1
Math1	ON	9	Math1				
Math2	ON	10	Math2				
Math3	ON	11	Math3				
Math4	ON	12	Math4				
Math5	ON	13	Math5				
Math6	ON	14	Math6				
Math7	ON	15	Math7				
Math8	ON	16	Math8				

When the mapping mode is set to User, you can set how to map each waveform to the divided screens.

Set the waveform mapping mode (Auto, User).

Set the waveform color.

When computation mode is OFF: Blank
When computation mode is ON: Depending on the operator set for each computation, the setting is as follows.
When computation is defined: ON or OFF can be selected
When set to OFF: Blank

If FFT1 is set to ON, FFT1 appears in the Math7 position.
If FFT2 is set to ON, FFT2 appears in the Math8 position.

FFT1	-		
FFT2	-		

Label: Blank

Map: -

Set the FFT waveform color.

Disp: Blank

8.2 Using the Snapshot and Clear Trace Features

This section explains how to use the snapshot feature (which retains the currently displayed waveforms on the screen) and the clear trace feature (which clears all displayed waveforms).

► [Features Guide: “Snapshot \(SNAPSHOT\)”](#)
[“Clear Trace \(CLEAR TRACE\)”](#)

Snapshot (SNAPSHOT)

Press **SNAPSHOT** to retain the currently displayed waveform on the screen as a snapshot waveform in white. Snapshot waveforms remain on the screen until you execute a clear trace operation.

Clear Trace (CLEAR TRACE)

Press **CLEAR TRACE** to clear all the waveforms that are displayed on the screen.

Note

Click **SHIFT+SNAPSHOT** to clear only the snapshot waveforms.

9.1 Configuring the Bar Graph Display

This section explains the following settings for displaying bar graphs. These settings are available on models with the harmonic measurement (/G5) option.

- Bar graph display format
- Bar graph number
- Measurement function
- Element
- Bar graph display range (displayed harmonics)
- Turning the numeric data display on and off
- Marker position (harmonic)

► [Features Guide: “Bar Graph Display \(Option\)”](#)

BAR SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the BAR SETTING menu.

BAR SETTING	
Format	Set the display format (1 (no windows), 2, 3).
Item No	Set the bar graph number (1-3).
Function	Set the measurement function (U, I, P, S, Q, λ , Φ , ΦU , ΦI , Z, Rs, Xs, Rp, Xp).
Element	Set the element (Element 1-Element 4).
Start Order	Set the bar graph display range.
End Order	<ul style="list-style-type: none"> • The display's starting harmonic order (0-490) • The display's ending harmonic order (10-500)
Numeric	You can set the range to any value provided that the end harmonic order is larger than the start harmonic order by 10 or more.
× Order	Turns the numeric data display on and off
+ Order	Set the harmonic order of the bar graph to measure with markers x and + (0-500).

If you press this soft key and select both × Order and + Order, you can change both orders while maintaining the relationship between the two.

10.1 Configuring the Vector Display

This section explains the following settings for displaying vectors. These settings are available on models with the harmonic measurement (/G5) option.

- Vector display format
- Vector number
- Element and wiring unit
- Zooming vectors
- Turning the numeric data display on and off

► [Features Guide: “Vector Display \(Option\)”](#)

VECTOR SETTING Menu

Use the **DISPLAY MODE** and **DISPLAY SETTING** keys as explained in section 5.1 to display the VECTOR SETTING menu.

VECTOR SETTING	
Format	Set the display format (1 (no windows), 2).
Item No	Set the vector number (1, 2).
Vector Object	Set the element and wiring unit (Element 1-Element 4, ΣA , ΣB).
U Mag	Set the magnification of vectors of the fundamental waves U(1) and I(1) (0.100-100.000). The value that indicates the size of the vector display's peripheral circle changes according to the zoom factor, and the size of the vectors that indicate U (1) and I (1) change accordingly as well. If you press this soft key to select both U Mag and I Mag, you can change both magnifications while maintaining the relationship between the two.
I Mag	
Numeric	Turns the numeric data display on and off
OFF ON	

11.1 Displaying X-Y Waveforms


This section explains the following settings for displaying X-Y waveforms.

- Turning the X-Y window display on and off
- Turning the X-Y waveform on and off and X-axis and Y-axis source waveforms
- Start and end points
- Turning the trace-clear-on-start on and off
- Main window's display ratio
- Window layout
- Turning combine display on and off
- Interpolation method
- The number of data points that are used to display waveforms

► [Features Guide: “Displaying X-Y Waveforms”](#)


X-Y Menu

1. Press **SHIFT+SETTING** (X-Y) to display the following menu.

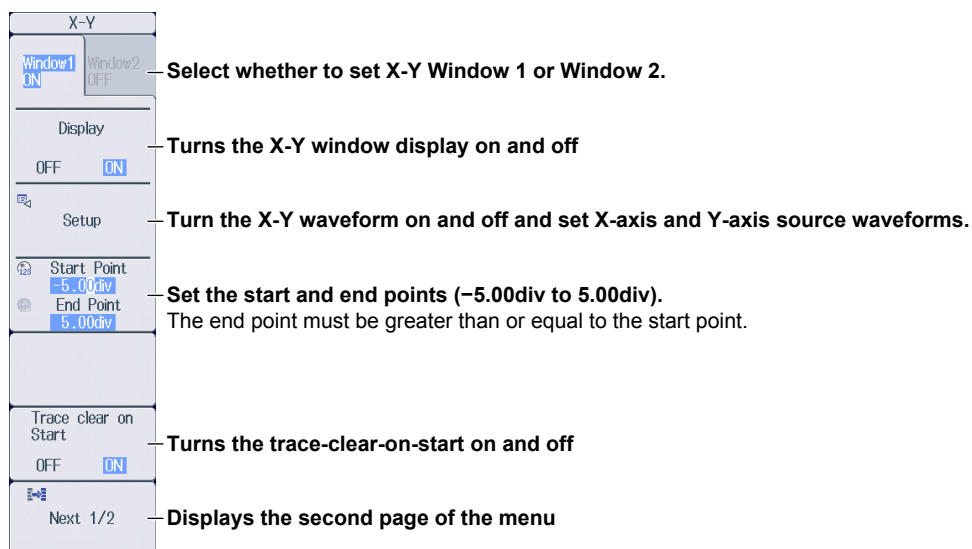

11.1 Displaying X-Y Waveforms


2. Press the **Next 1/2** soft key to display the 2/2 menu.

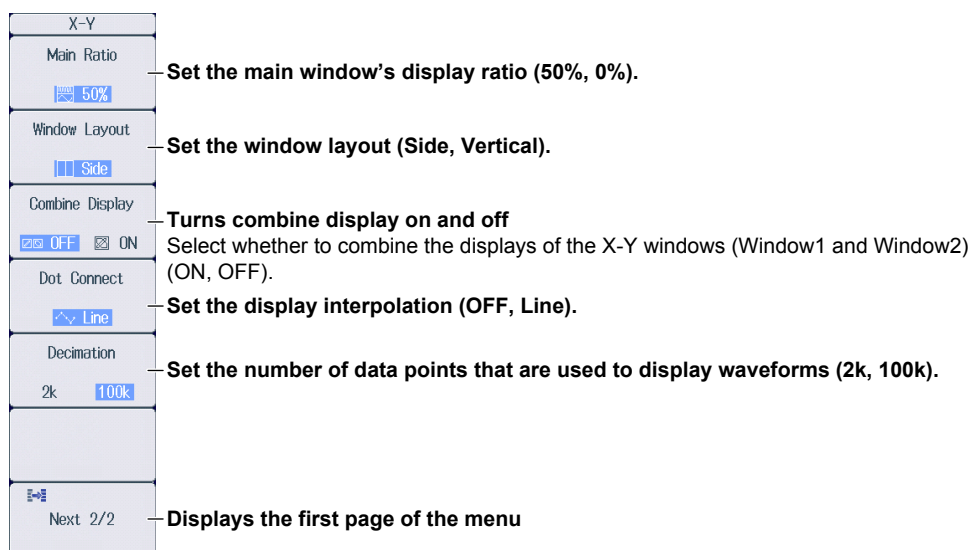


Turning the X-Y Waveform On and Off and Setting X-Axis and Y-Axis Source Waveforms

Press the **Setup** soft key to display the following screen.

**When X-Y Window 1 is selected,
Set the X-Y waveforms of XY1 to XY4.**

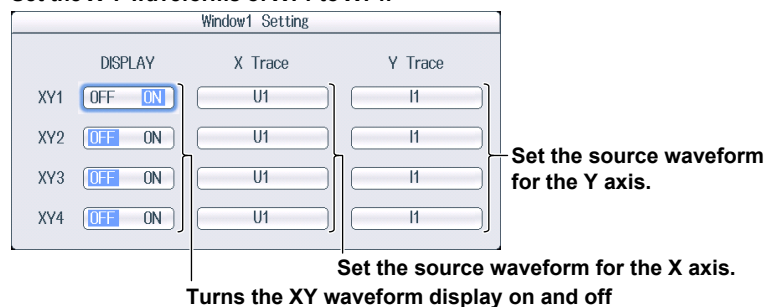

**When X-Y Window 2 is selected,
Set the X-Y waveforms of XY5 to XY8.**

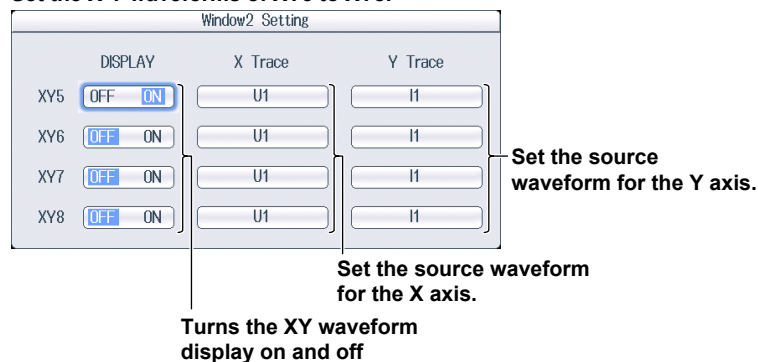

12.1 Zooming in on or out of Waveforms

This section explains the following settings for zooming in on or out of waveforms horizontally (time scale). For details on vertical zoom settings, see sections 2.1 to 2.6 or section 8.1.


- Turning the zoom window display on and off
- Zoom position and zoom box
- Zoom display format
- Zoom 2 source window
- Main window's display ratio
- Window layout
- Auto scrolling
- Zoom source waveform
- Changing the range for performing automated measurement of waveform parameters
- Zoom position using the zoom POSITION knob and magnification

► [Features Guide: “Zooming in on Waveforms”](#)


ZOOM Menu

1. Press **ZOOM** to display the following menu.
 - If you press **ZOOM** while no zoom window is displayed on the screen, zoom box 1 is automatically turned on (Z1 ON).
 - Set the menu items separately for zoom windows Zoom 1 and Zoom2.

Setting the Zoom 1 window

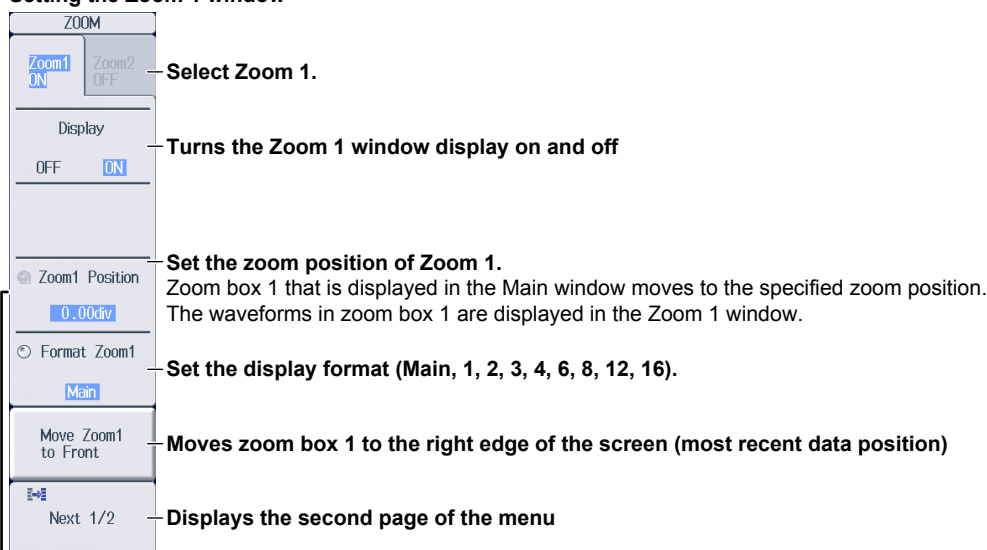

When both Zoom 1 and Zoom 2 window displays are on

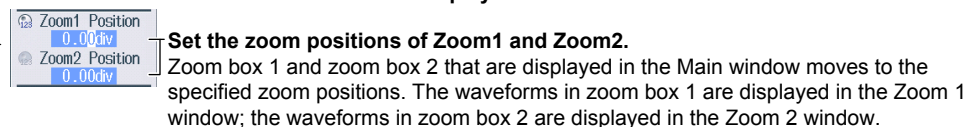

12.1 Zooming in on or out of Waveforms

Setting the Zoom 2 window

The screenshot shows the ZOOM menu with the following options and annotations:

- Zoom1 ON** and **Zoom2 ON**: Select Zoom 2.
- Display** (OFF/ON): Turns the Zoom 2 window display on and off.
- Zoom2 Source** (Main/Zoom1): Select the zoom source window for Zoom 2 (Main, Zoom 1). When Zoom 1 window is on, select Main or Zoom 1.
- Zoom2 Position** (0.00div): Set the zoom position of Zoom 2. Zoom box 2 that is displayed in the Main window moves to the specified zoom position. The waveforms in zoom box 2 are displayed in the Zoom 2 window.
- Format Zoom2** (Main, 1, 2, 3, 4, 6, 8, 12, 16): Set the display format (Main, 1, 2, 3, 4, 6, 8, 12, 16).
- Move Zoom2 to Front**: Moves zoom box 2 to the right edge of the screen (most recent data position). This is available when Zoom 2 Source (shown above) is set to Main.
- Next 1/2**: Displays the second page of the menu.

2. Press the **Next 1/2** soft key to display the 2/2 menu.

The screenshot shows the ZOOM menu page 2/2 with the following options and annotations:

- Main Ratio** (50%): Set the main window's display ratio (50%, 0%).
- Window Layout** (Side): Set the window layout (Side, Vertical).
- Auto Scroll**: Configure auto scrolling.
- Allocation**: Set the zoom source waveforms.
- Fit Measure Range to Zoom1**: Change the range for performing automated measurement of waveform parameters. The range over which automated measurement of waveform parameters is performed is set to the zoom range of Zoom1 when the Zoom 1 window is on and the zoom range of Zoom2 when the Zoom 2 window is on.
- Next 2/2**: Displays the first page of the menu.

When both Zoom 1 and Zoom 2 window displays are on

The diagram shows a flow from the **Fit Measure Range** option in the menu to a selection screen with two options: **Fit to Zoom1** and **Fit to Zoom2**. A bracket indicates that the user should select which zoom range: Zoom 1 or Zoom 2.

Setting Auto Scrolling (Auto Scroll)

Press the **Auto Scroll** soft key to display the following menu.

Auto Scroll

Target

Zoom1 Zoom2

Speed

4

▶▶

▶

■

◀

◀◀

Select the zoom box to auto scroll.

When both Zoom 1 and Zoom 2 window displays are on, select Zoom 1 or Zoom 2.

Set the scroll speed (1-10).

Moves to the right edge of the Main window

Starts scrolling to the right

Stops auto scrolling

Starts scrolling to the left

Moves to the left edge of the Main window

Allocating Zoom Source Waveforms (Allocation)

Press the **Allocation** soft key to display the following screen.

Allocation			
✓U1	-	-	-
✓I1	-	-	-
✓P1	-	-	-
✓U2	-	-	-
✓I2	-	-	-
✓P2	-	-	-
✓AUX5	-	-	-
✓AUX6	-	-	-
✓Math1	-	-	-
✓Math2	-	-	-
✓Math3	-	-	-
✓Math4	-	-	-
✓Math5	-	-	-
✓Math6	-	-	-
✓Math7	-	-	-
✓Math8	-	-	-


Select the zoom source waveforms.

The waveforms that can be selected are displayed.

Setting the Magnification (MAG knob)

Use the **MAG** knob to set the magnification.

- The MAG knob controls the waveforms in the zoom window whose corresponding indicator, Z1 or Z2, is illuminated.
- The MAG knob has a push switch. Push the knob to illuminate the Z1 indicator, Z2 indicator, or both indicators. When both the Z1 and Z2 indicators are illuminated, you can set both zoom windows to the same magnification at the same time.

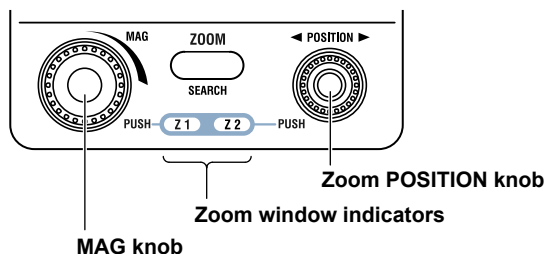

Setting the Zoom Position (zoom POSITION knob)

Turn the zoom **POSITION** knob to set the zoom position.

- The zoom POSITION knob controls the waveforms in the zoom window whose corresponding indicator, Z1 or Z2, is illuminated.
- The zoom POSITION knob has a push switch. Push the knob to illuminate the Z1 indicator, Z2 indicator, or both indicators. When both the Z1 and Z2 indicators are illuminated, you can set both zoom windows to the same zoom position at the same time.

13.1 Measuring with Horizontal Cursors


This section explains the following settings for measuring with horizontal cursors:

- Cursor type
- Source waveform
- Moving the cursors
- Measurement items
- Windows that cursor measurements will be performed in

► **Features Guide: “Horizontal Cursors (Horizontal) - T-Y waveforms”**
“Horizontal Cursors (Horizontal) (X-Y)”
“Turning the X-Y Window Display On and Off (Display)”

CURSOR Horizontal Menu

Press **CURSOR**, the **Type** soft key, and then the **Horizontal** soft key to display the following menu.

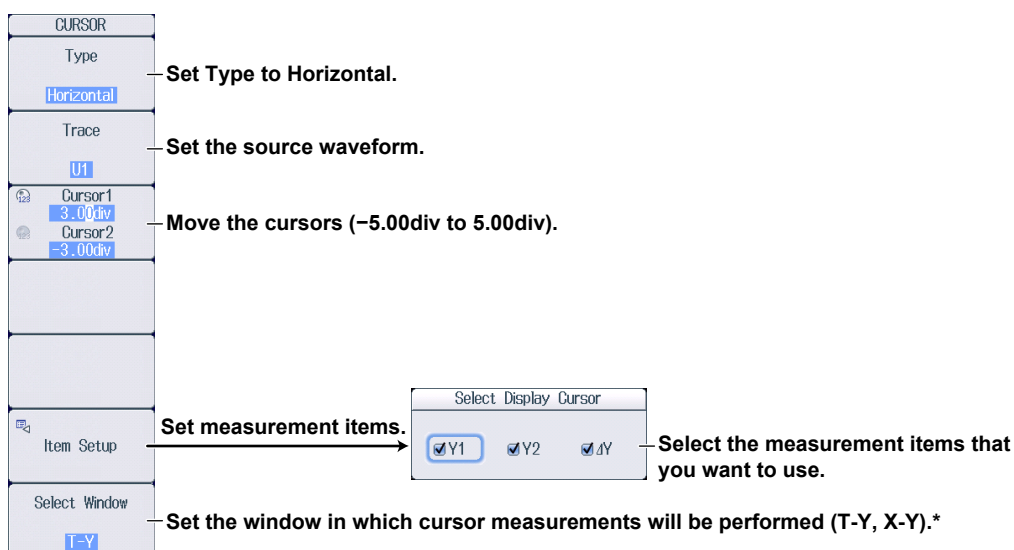

* This is available when the X-Y window display is turned on.

Setting the Source Waveform (Trace)

The waveforms that you can select differ depending on the window that cursor measurements will be performed in.

- T-Y: U1 to U4, I1 to I4, P1 to P4, AUX3 to AUX8, Math1 to Math8
- X-Y: XY1 to XY8

13.2 Measuring with Vertical Cursors


This section explains the following settings for measuring with vertical cursors:

- Cursor type
- Source waveform
- Moving the cursors
- Jumping the cursors
- Measurement items
- Windows that cursor measurements will be performed in

► **Features Guide: “Vertical Cursors (Vertical) - T-Y waveforms”**
“Vertical Cursors (Vertical) (X-Y)”
“Turning the X-Y Window Display On and Off (Display)”
“Record Length (Record Length)”

CURSOR Vertical Menu

Press **CURSOR**, the **Type** soft key, and then the **Vertical** soft key to display the following menu.

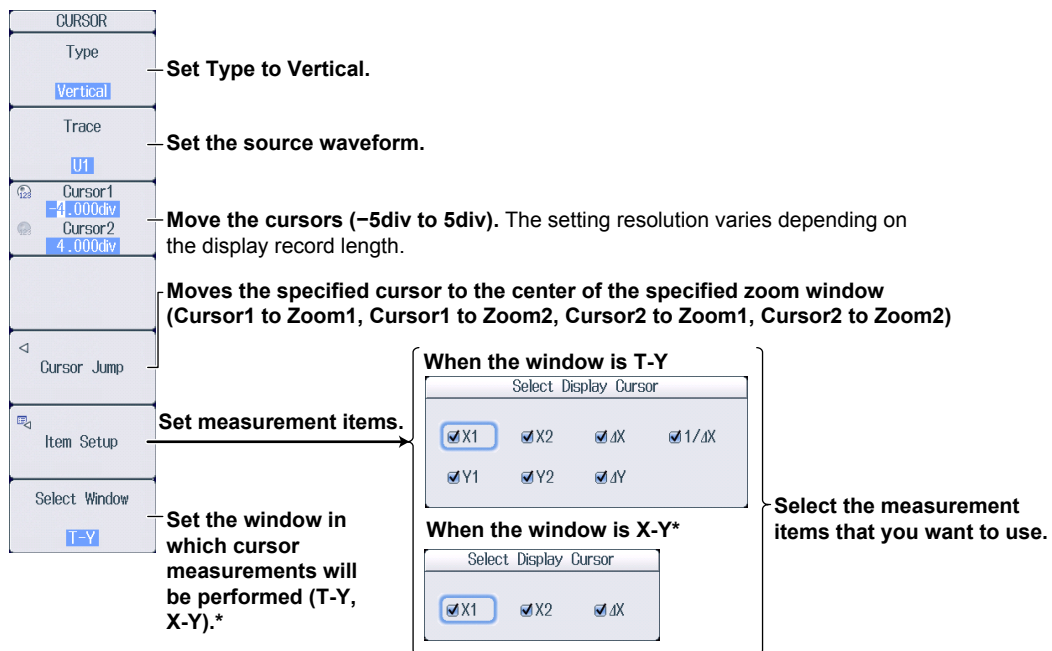

* This is available when the X-Y window display is turned on.

Setting the Source Waveform (Trace)

The waveforms that you can select differ depending on the window that cursor measurements will be performed in.

- T-Y: All, U1 to U4, I1 to I4, P1 to P4, AUX3 to AUX8, Math1 to Math8
- X-Y: XY1 to XY8

13.3 Measuring with Marker Cursors (Marker)

This section explains the following settings for measuring with marker cursors.

- Cursor type
- Source waveform
- Moving the cursors
- Jumping the cursors
- Marker display format
- Measurement items
- Windows that cursor measurements will be performed in

► Features Guide: “Marker Cursors (Marker) - T-Y waveforms”

“Marker Cursors (Marker) (X-Y)”

“Marker Cursors (Marker) (FFT)”

“Turning the X-Y Window Display On and Off (Display)”

“Turning FFT On and Off (Display)”

“Record Length (Record Length)”

“Start Point and Number of FFT Points (Start Point and FFT Points)”

CURSOR Marker Menu

Press **CURSOR**, the **Type** soft key, and then the **Marker** soft key to display the following menu.

The diagram illustrates the CURSOR Marker Menu and its sub-menus. The main menu is shown on the left, with arrows pointing to specific options and their functions. The sub-menus are shown on the right, with arrows pointing to specific options and their functions.

CURSOR Marker Menu:

- Type** (Set the cursor type to Marker.)
- Marker #** (Select the marker cursor to use (Marker1 X, Marker2 +, Marker3 Y, Marker4 Y).)
- Trace** (Set the source waveform.)
- Position** (Move the cursors (-5div to 5div). The setting resolution varies depending on the display record length. The setting resolution when the window is FFT varies depending on the number of FFT points.)
- Cursor Jump** (Moves the specified cursor to the center of the specified zoom window (to Zoom1, to Zoom2))
- Item & Marker Form** (Set measurement items.)
- Select Window** (Set the window in which cursor measurements will be performed (T-Y, X-Y, FFT).*)

When the Source Window is T-Y or FFT*

Select Display Cursor

Marker Form: Mark, Line

Set the marker display format (Mark, Line).

Display Item:

<input checked="" type="checkbox"/> X1	<input checked="" type="checkbox"/> X2	<input checked="" type="checkbox"/> X3	<input checked="" type="checkbox"/> X4
<input checked="" type="checkbox"/> d(X2-X1)	<input checked="" type="checkbox"/> d(X3-X1)	<input checked="" type="checkbox"/> d(X4-X1)	
<input type="checkbox"/> d(X3-X2)	<input type="checkbox"/> d(X4-X2)	<input type="checkbox"/> d(X4-X3)	
<input checked="" type="checkbox"/> Y1	<input checked="" type="checkbox"/> Y2	<input checked="" type="checkbox"/> Y3	<input checked="" type="checkbox"/> Y4
<input checked="" type="checkbox"/> d(Y2-Y1)	<input checked="" type="checkbox"/> d(Y3-Y1)	<input checked="" type="checkbox"/> d(Y4-Y1)	
<input type="checkbox"/> d(Y3-Y2)	<input type="checkbox"/> d(Y4-Y2)	<input type="checkbox"/> d(Y4-Y3)	

Select the measurement items that you want to use.

When the window is X-Y*

Select Display Cursor

<input checked="" type="checkbox"/> X1	<input checked="" type="checkbox"/> X2	<input checked="" type="checkbox"/> X3	<input checked="" type="checkbox"/> X4
<input checked="" type="checkbox"/> Y1	<input checked="" type="checkbox"/> Y2	<input checked="" type="checkbox"/> Y3	<input checked="" type="checkbox"/> Y4
<input checked="" type="checkbox"/> T1	<input checked="" type="checkbox"/> T2	<input checked="" type="checkbox"/> T3	<input checked="" type="checkbox"/> T4
<input checked="" type="checkbox"/> d(T2-T1)	<input checked="" type="checkbox"/> d(T3-T1)	<input checked="" type="checkbox"/> d(T4-T1)	

* This is available when the X-Y window display or FFT window display is turned on.

Setting the Source Waveform (Trace)

The waveforms that you can select differ depending on the window that cursor measurements will be performed in.

- T-Y: OFF, U1 to U4, I1 to I4, P1 to P4, AUX3 to AUX8, Math1 to Math8
- X-Y: OFF, XY1 to XY8
- FFT: OFF, FFT1, FFT2

13.4 Measuring with Angle Cursors (Degree)

This section explains the following settings for measuring with angle cursors. You can use angle cursors when the T-Y window is displayed.

- Cursor type
- Source waveform
- Moving the cursors
- Zero and end reference angles
- Jumping the cursors
- Measurement items
- Reference angle
- Windows that cursor measurements will be performed in

► **Features Guide: “Angle Cursors (Degree) - T-Y waveforms”**
“Record Length (Record Length)”

CURSOR Degree Menu

1. Press **CURSOR**, the **Select Window** soft key, and then the **T-Y** soft key.
2. Press the **Type** soft key and then the **Degree** soft key to display the following menu.

The image shows the CURSOR Degree Menu and the Select Display Cursor dialog. The menu is a vertical list of options: CURSOR, Type, Trace, Cursor1, Cursor2, Ref1, Ref2, Cursor Jump, Item & RefValue, and Select Window. The Type option is highlighted with 'Degree' below it. The Trace option is highlighted with 'U1' below it. The Cursor1 option is highlighted with '-4.000div' below it. The Cursor2 option is highlighted with '4.000div' below it. The Ref1 option is highlighted with '-2.000div' below it. The Ref2 option is highlighted with '2.000div' below it. The Cursor Jump option is highlighted with '<' below it. The Item & RefValue option is highlighted with 'Item & RefValue' below it. The Select Window option is highlighted with 'T-Y' below it. The Select Display Cursor dialog is shown to the right of the Item & RefValue option. It has a RefValue field set to 360. It has a Display Item section with checkboxes for X1, X2, ΔX, Y1, Y2, and ΔY. X1, X2, ΔX, Y1, Y2, and ΔY are all checked. X1 is highlighted with a blue box.

CURSOR

Type
Degree

Trace
U1

Cursor1
-4.000div

Cursor2
4.000div

Ref1
-2.000div

Ref2
2.000div

Cursor Jump
<

Item & RefValue
Item & RefValue

Select Window
T-Y

Select Display Cursor

RefValue 360

Display Item

☒ X1 ☒ X2 ☒ ΔX

☒ Y1 ☒ Y2 ☒ ΔY

13.5 Measuring with Horizontal and Vertical Cursors (H & V)

This section explains the following settings for measuring with horizontal and vertical cursors:

- Cursor type
- Source waveform
- Moving the vertical cursors
- Moving the horizontal cursors
- Jumping the cursors
- Measurement items
- Windows that cursor measurements will be performed in

► **Features Guide:** “Horizontal and Vertical Cursors (H & V) - T-Y waveforms”
 “Horizontal and Vertical Cursors (H & V) (X-Y)”
 “Turning the X-Y Window Display On and Off (Display)”
 “Record Length (Record Length)”

CURSOR H & V Menu

Press **CURSOR**, the **Type** soft key, and then the **H & V** soft key to display the following menu.

The screenshot shows the CURSOR H & V menu with the following options and annotations:

- CURSOR**: The main menu title.
- Type**: Set Type to H & V.
- Trace**: Set the source waveform.
- V-Cursor1**: Move the vertical cursors (–5div to 5div). The setting resolution varies depending on the display record length.
- V-Cursor2**: Move the vertical cursors (–5div to 5div). The setting resolution varies depending on the display record length.
- H-Cursor1**: Move the horizontal cursors (–5.00div-5.00div).
- H-Cursor2**: Move the horizontal cursors (–5.00div-5.00div).
- Cursor Jump**: Moves the specified cursor to the center of the specified zoom window (Cursor1 to Zoom1, Cursor1 to Zoom2, Cursor2 to Zoom1, Cursor2 to Zoom2).
- Item Setup**: Set measurement items. When the window is T-Y, Select Display Cursor: ☒ X1, ☒ X2, ☒ ΔX, ☒ 1/ΔX, ☒ Y1, ☒ Y2, ☒ ΔY. When the window is X-Y*, Select Display Cursor: ☒ X1, ☒ X2, ☒ ΔX, ☒ Y1, ☒ Y2, ☒ ΔY. Select the measurement items that you want to use.
- Select Window**: Window in which cursor measurements will be performed (T-Y, X-Y)*.

* This is available when the X-Y window display is turned on.

Setting the Source Waveform (Trace)

The waveforms that you can select differ depending on the window that cursor measurements will be performed in.

- T-Y: U1 to U4, I1 to I4, P1 to P4, AUX3 to AUX8, Math1 to Math8
- X-Y: XY1 to XY8

13.6 Measuring with Peak Cursors (Peak)

This section explains the following settings for measuring with peak cursors. You can use peak cursors when the FFT window is displayed.

- Cursor type
- Two measurement ranges
- Measurement items
- Windows that cursor measurements will be performed in

► **Features Guide: “Peak Cursors (Peak)”**

“Turning FFT On and Off (Display)”

“Start Point and Number of FFT Points (Start Point and FFT Points)”

CURSOR Peak Menu

1. Press **CURSOR**, and then press the **Select Window** soft key and then the FFT soft key.
2. Press the **Type** soft key and then the Peak soft key to display the following menu.

CURSOR	
Type	Peak
FFT1 Range1	-5.00div
FFT1 Range2	5.00div
FFT2 Range1	-5.00div
FFT2 Range2	5.00div
Item Setup	
Select Window	FFT

Set Type to Peak.

Set the FFT1 measurement time period (-5div to 5div). The setting resolution varies depending on the number of FFT points.

Set the FFT2 measurement time period (-5div to 5div). The setting resolution varies depending on the number of FFT points.

Set measurement items.

Set Select Window to FFT.

Select Display Cursor	
<input checked="" type="checkbox"/> F1	<input checked="" type="checkbox"/> F2
<input checked="" type="checkbox"/> Y1	<input checked="" type="checkbox"/> Y2

Select the measurement items that you want to use.

14.1 Automatically Measuring Waveform Parameters

This section explains the following settings for automatically measuring waveform parameters.

- Turning automated measurement on and off
- Source waveform and measurement items
- Measurement time period
- Turning cycle mode on and off
- Parameter details
- Delay settings

► **Features Guide: “Automated Measurement of Waveform Parameters”**
“Record Length (Record Length)”


MEASURE Menu

Press **MEASURE**, the **Mode** soft key, and then the **ON** soft key to display the following menu.

MEASURE	
Mode	Set Mode to ON.
ON	
◀ Measure Setup	Set the source waveform and measurement items.
Time Range1 5.00div	Set the measurement time period (–5div to 5div). The setting resolution varies depending on the display record length. Time period 2 (Time Range2) must be greater than or equal to Time period 1 (Time Range1). The maximum number of data points that are measured is 100 Mpoint from Time Range 1.
Time Range2 5.00div	
1-Cycle Mode	Turns cycle mode on and off If the measurement time period (the spacing between Time Range1 and Time Range2) is less than 1 cycle, the measured value will be “*****.”
OFF ON	


Setting the Source Waveform and Configuring the Measurement Items (Measure Setup)

1. Press the **Measure Setup** soft key to display the following menu.

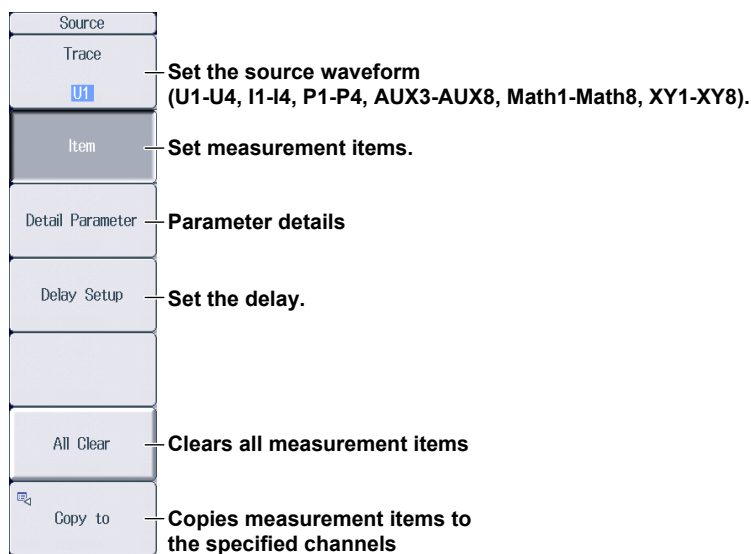


Setting Measurement Items (Item)


2. Press the **Item** soft key to display the following screen.
- When the Source Waveform Is U1 to U4, I1 to I4, P1 to P4, AUX3 to AUX8, Math1 to Math8

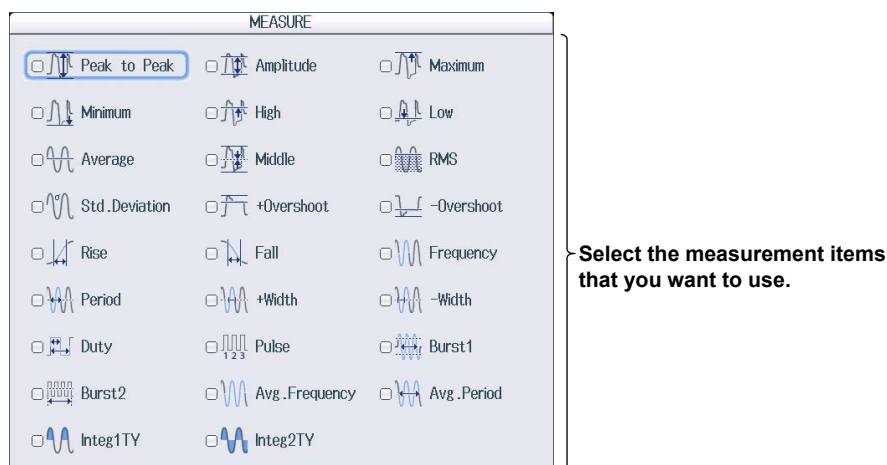


- When the Source Waveform Is XY1 to XY8

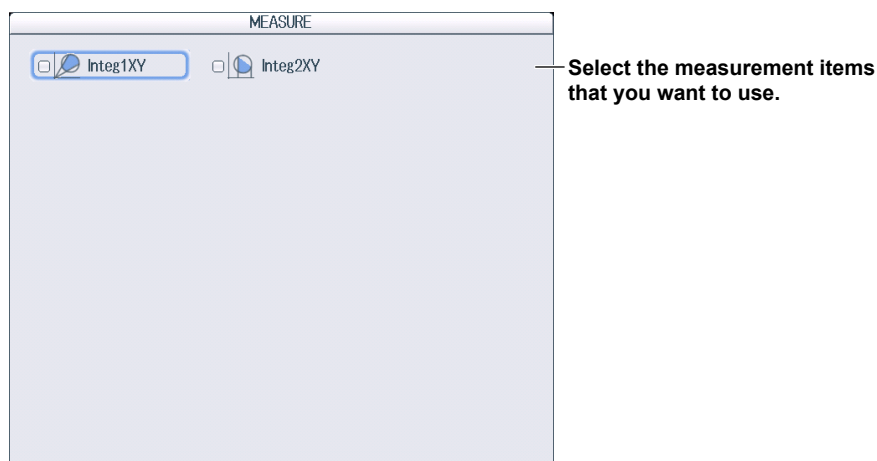

2. Press the **Detail Parameter** soft key to display the following screen.

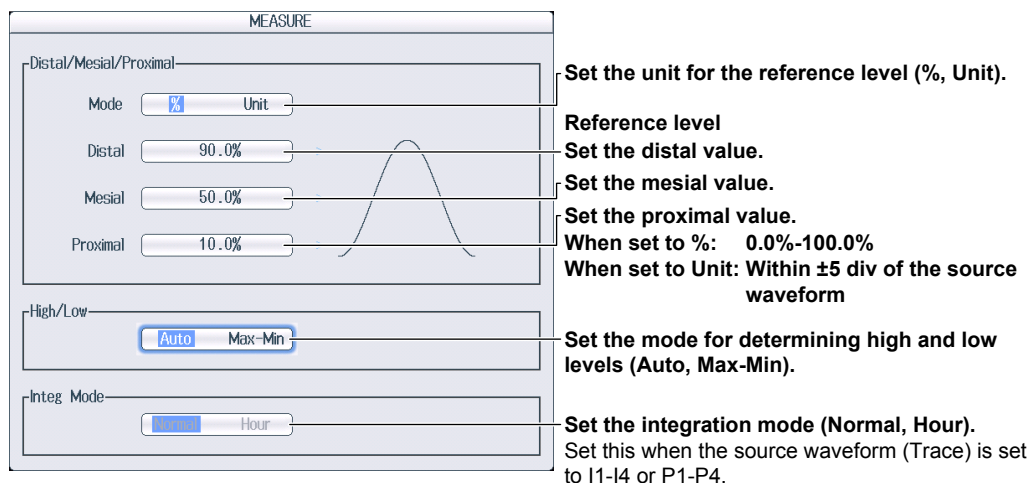


2. Press the **Delay Setup** soft key to display the following screen.

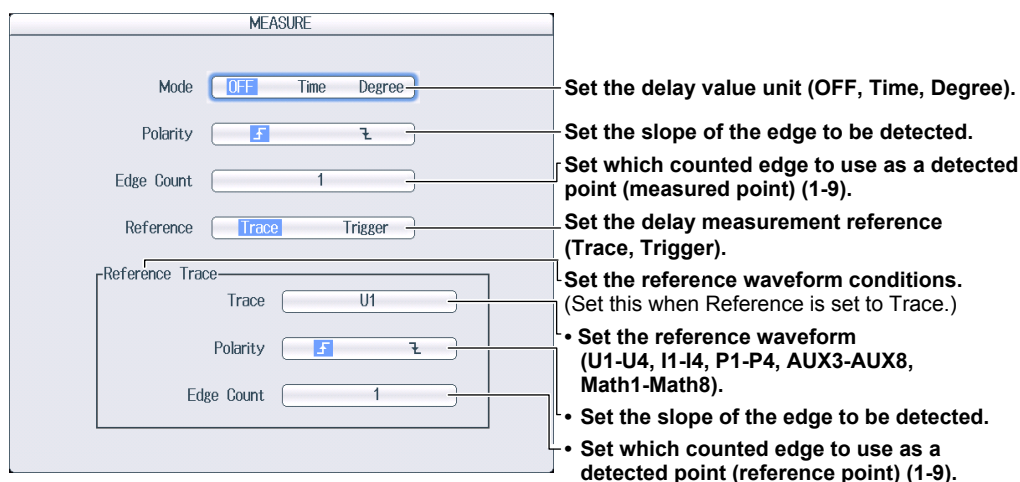

2. Press the **Copy to** soft key to display the following screen.

Copies the contents specified by measurement item (Item) to the selected waveforms (Trace) (U1-U4, I1-I4, P1-P4, AUX3-AUX8, Math1-Math8)

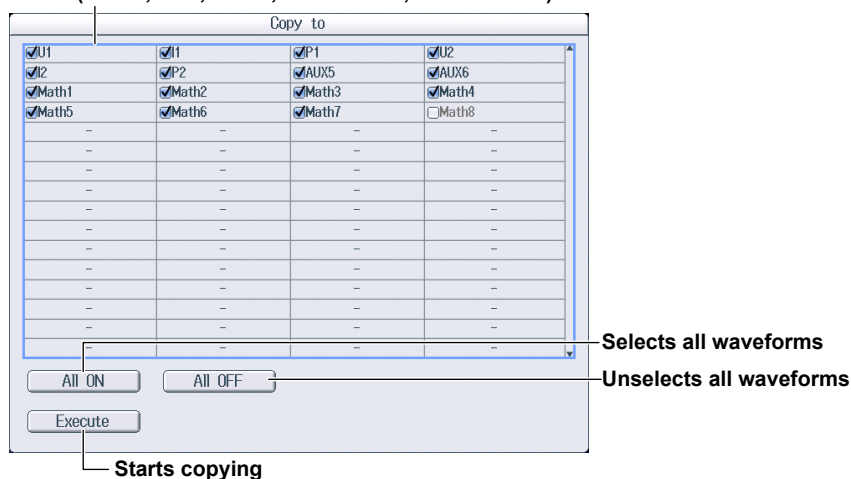

14.2 Performing Normal Statistical Processing


This section explains the following settings for performing normal statistical processing on automatically measured waveform parameters.

- Normal statistical processing

► [Features Guide: “Normal Statistical Processing \(Statistics\)”](#)

MEASURE Menu

Press **MEASURE**, the **Mode** soft key, and then the **Statistics** soft key to display the following menu.

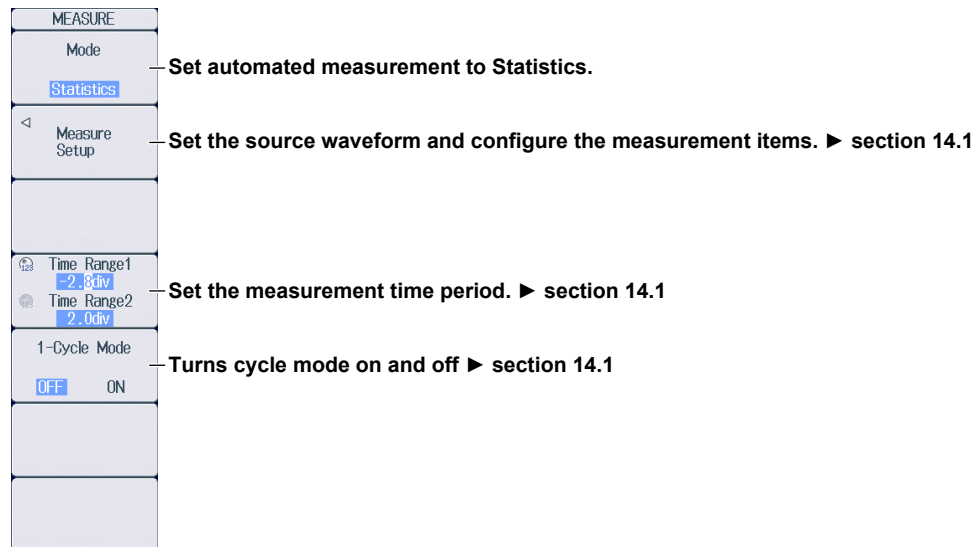

14.3 Performing Cyclic Statistical Processing


This section explains the following settings for performing cyclic statistical processing on automatically measured waveform parameters.

- Cyclic statistical processing
- Cycle trace (source waveform for determining the cycle)
- Result display

► [Features Guide: “Cyclic Statistical Processing \(Cycle Statistics\)”](#)

MEASURE Menu

Press **MEASURE**, the **Mode** soft key, and then the **Cycle Statistics** soft key to display the following menu.

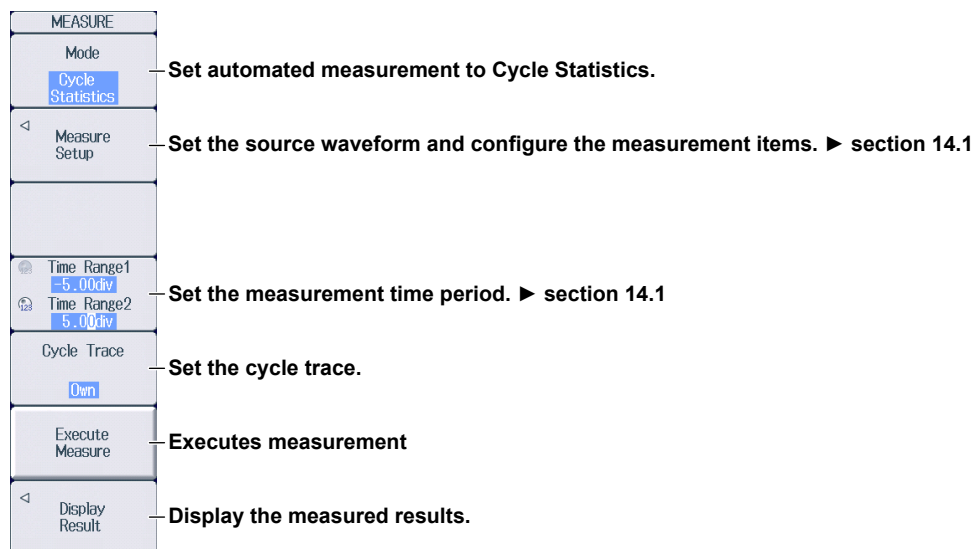

Setting the Cycle Trace (Cycle Trace)

U1 to U4, I1 to I4, P1 to P4, AUX3 to AUX8, Math1 to Math8:

The PX8000 automatically measures the waveform parameters of all the source waveforms and performs statistical processing on the measured values once per cycle of the specified waveform.

Own:

The PX8000 determines the cycle of each source waveform. It then automatically measures the waveform parameters and performs statistical processing once per cycle of each waveform. However, if multiple waveforms with different cycles are measured, the number of iterations of automated measurement of waveform parameters and statistical processing performed on all waveforms is equal to the number of cycles in the slowest waveform.

Displaying the Measured Results (Display Result)

Press the **Display Result** soft key to display the following screen.

- ↑: Displayed next to the maximum value of each measurement item.
↓: Displayed next to the minimum value of each measurement item.

Cycle Statistics					Jump & Sort	
	Min(AUX5)	High(AUX5)	Low(AUX5)	Avg(AUX5)	<	Sort
3	-1.33333mV	994.667mV	2.00000mV	498.805mV		Forward
4	0.00000V ↑	994.667mV	2.00000mV	498.897mV		
5	-2.66667mV	993.333mV ↓	2.00000mV	498.862mV		
6	-1.33333mV	994.667mV	2.00000mV	498.813mV		
7	-2.66667mV	994.667mV	2.00000mV	499.126mV		
8	-4.00000mV	994.667mV	2.00000mV	499.108mV		
9	-2.66667mV	994.667mV	2.00000mV	498.927mV		
10	-4.00000mV	994.667mV	3.33333mV ↑	499.148mV		
11	-1.33333mV	993.333mV	2.00000mV	499.110mV		
12	-2.66667mV	994.667mV	2.00000mV	499.092mV		
13	-1.33333mV	996.000mV ↑	2.00000mV	499.123mV		
14	-2.66667mV	994.667mV	2.00000mV	499.216mV		
15	-1.33333mV	994.667mV	2.00000mV	499.269mV		
16	-5.33333mV	994.667mV	3.33333mV	499.067mV		Statistics Max
17	0.00000V	996.000mV	2.00000mV	499.063mV		
18	-2.66667mV	994.667mV	666.667uV ↓	498.896mV		
19	-1.33333mV	994.667mV	3.33333mV	499.128mV		
20	-2.66667mV	994.667mV	2.00000mV	498.854mV		
21	-6.66667mV ↓	994.667mV	666.667uV	498.828mV		
22	-2.66667mV	994.667mV	2.00000mV	498.858mV		
23	-1.33333mV	994.667mV	666.667uV	498.941mV		
24	-2.66667mV	994.667mV	2.00000mV	498.888mV		
25	-1.33333mV	993.333mV	666.667uV	498.885mV		
26	-1.33333mV	993.333mV	3.33333mV	499.135mV		
27	-2.66667mV	994.667mV	2.00000mV	499.066mV		
28	-4.00000mV	994.667mV	666.667uV	498.890mV		
29	-1.33333mV	993.333mV	2.00000mV	499.077mV		
30	0.00000V	994.667mV	2.00000mV	499.372mV ↑		

If scroll bars are displayed, you can press the arrow keys (▲, ▼, ◀, ▶) to scroll the list.
You can scroll vertically also using the jog shuttle.

15.1 Performing Addition, Subtraction, Multiplication, and Division

This section explains the following settings for performing addition, subtraction, multiplication, and division.

- Computation
Operator (+, −, *, /), computation source waveform, unit, label, turning the waveform display on and off
- Scaling
Math waveform to scale (computed waveform), scaling mode, upper and lower limits of the display range
- Computation start and end points

► **Features Guide: “Basic Arithmetic (S1+S2, S1-S2, S1*S2, and S1/S2)”**
“Scaling Mode (Scaling Mode)”
“Record Length (Record Length)”

MATH Menu

Press **MATH** to display the following menu.

The MATH menu is shown on the left, and the Setup screen is on the right. Arrows point from the MATH menu options to the Setup screen and to descriptive text.

- MATH**
- Mode**
OFF **ON** → **Set Mode to ON.**
- Math Setup** → **Set the computation.**
- Select Math Trace**
1 → **Set the scaling.**
- Scaling Mode**
Auto **Manual** → **Set the scaling mode (Auto, Manual).**
- Upper**
2.5000 → **Set the upper and lower limits of the display range (−9.9999E+30-9.9999E+30).**
- Lower**
−2.5000
- Start Point**
−5.00div → **Set this when the scaling mode is Manual.**
- End Point**
5.00div → **Set the computation start and end points (−5div to 5div).**
The setting resolution varies depending on the display record length. The end point must be greater than or equal to the start point. Note that there is a limitation in the number of data points that is used depending on the number of equations to be computed. Not all the data points may be used.
- Next 1/2**

The Setup screen on the right shows Math1 through Math8, each with an OFF button.

Configuring Computations (Math Setup)

1. Press the **Math Setup** soft key.
2. Press a soft key from **Math1** to **Math8** to display the following screen.

The Math1 setup screen is shown with the following fields and annotations:

- Operation**: S1 + S2 → **Select the operation (S1+S2, S1-S2, S1*S2, S1/S2).**
- Source1**: U1
- Source2**: I1 → **Select the computation source waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8, Math1-Math7).**
- Unit**: → **Set the unit.**
- Label**: Math1 → **Set the label.**
- Display**: OFF **ON** → **Turns the waveform display on and off**

15.2 Performing Binary Conversion


This section explains the following settings for performing binary conversions:

- Computation
Function (Bin(S1)), computation source waveform, threshold level, unit, label, turning the waveform display on and off
- Scaling
- Computation start and end points

► Features Guide: “Binary Conversion (Bin (S1))”


MATH Menu

Press **MATH** to display the following menu.

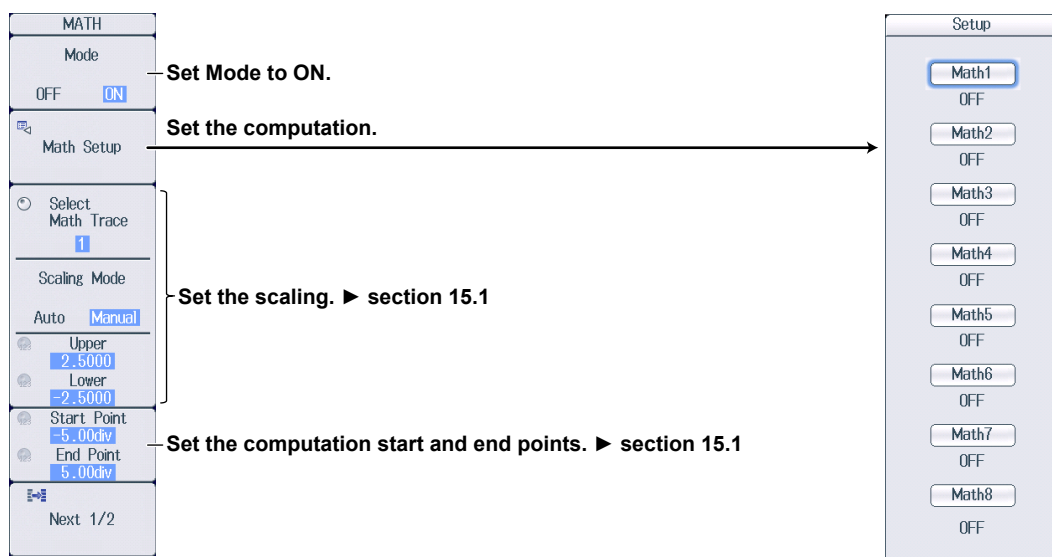

Configuring Computations (Math Setup)

1. Press the **Math Setup** soft key.
2. Press a soft key from **Math1** to **Math8** to display the following screen.

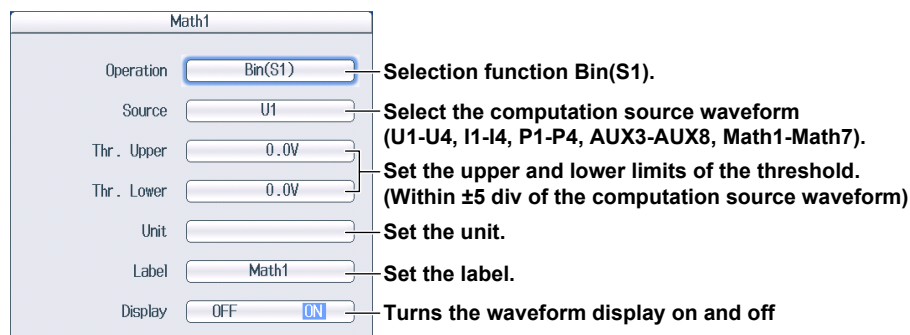

15.3 Shifting the Phase


This section explains the following settings for shifting the phase:

- Computation
Function (Shift(S1)), computation source waveform, shift range, unit, label, turning the waveform display on and off
- Scaling
- Computation start and end points

► [Features Guide: “Phase Shift \(Shift \(S1\)\)”](#)
[“Record Length \(Record Length\)”](#)


MATH Menu

Press **MATH** to display the following menu.

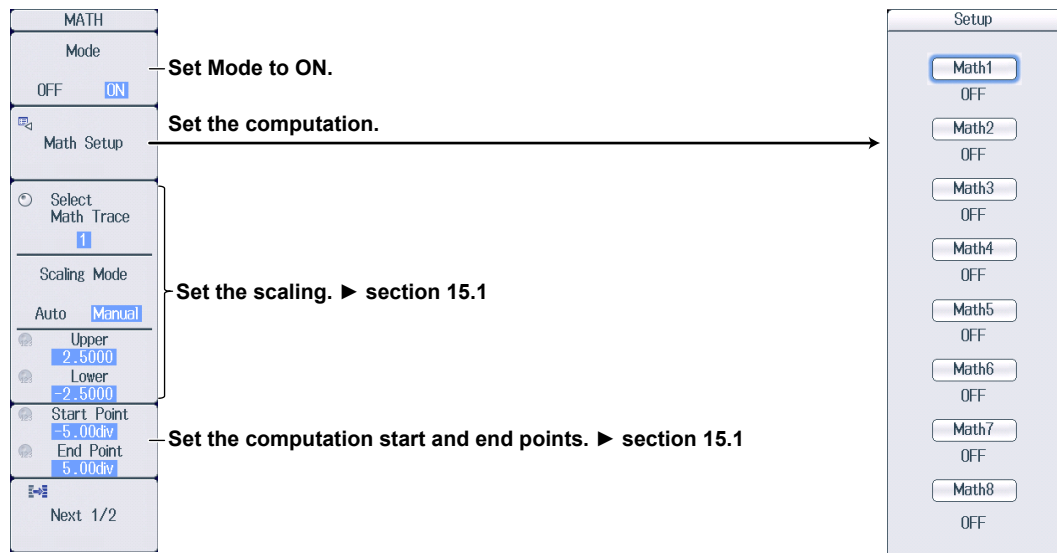

Configuring Computations (Math Setup)

1. Press the **Math Setup** soft key.
2. Press a soft key from **Math1** to **Math8** to display the following screen.

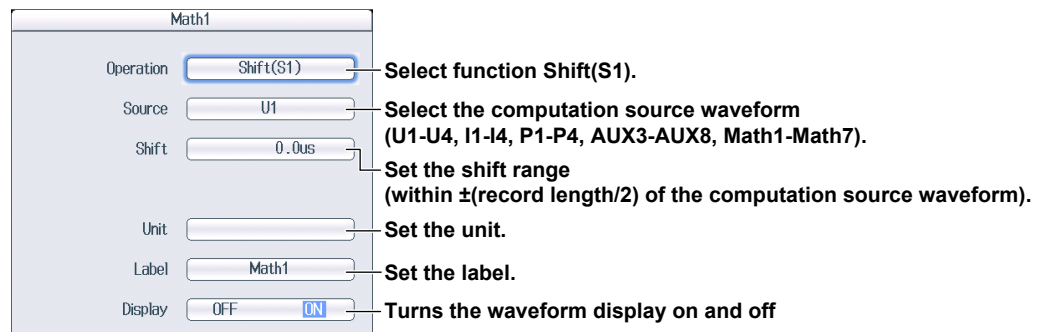

15.4 Displaying the Power Spectrum

This section explains the following settings for performing FFT and displaying the power spectrum.

- Computation
Function (PS(S1)), computation source waveform, unit, label, turning the waveform display on and off
- Scaling
- Computation start point
- FFT

► [Features Guide: “Power Spectrum \(PS \(S1\)\)”](#)

MATH Menu

Press **MATH** to display the following menu.

The diagram shows the **MATH** menu on the left and the **Setup** sub-menu on the right. Arrows indicate the flow from the **MATH** menu to the **Setup** sub-menu for various settings.

MATH Menu:

- Mode:** OFF, ON. **Set Mode to ON.**
- Math Setup:** **Set the computation.**
- Select Math Trace:** 1
- Scaling Mode:** Auto, Manual. **Set the scaling. ► section 15.1**
- Upper:** 2.5000
- Lower:** -2.5000
- Start Point:** -5.00div. **Set the computation start point. ► section 15.1**
- End Point:** 5.00div. **Set the start point of the FFT. The number of data points to use in the FFT (FFT points) is set on another menu.**
- Next 1/2:** **Set the number of FFT points. ► section 15.5**
- Displays the second page of the menu ► section 15.5**

Setup Sub-menu:

- Math1:** OFF
- Math2:** OFF
- Math3:** OFF
- Math4:** OFF
- Math5:** OFF
- Math6:** OFF
- Math7:** OFF
- Math8:** OFF

Configuring Computations (Math Setup)

1. Press the **Math Setup** soft key.
2. Press a soft key from **Math1** to **Math8** to display the following screen.

The diagram shows the **Math1** setup screen with the following fields and instructions:

- Operation:** PS(S1). **Select function PS(S1).**
- Source:** U1. **Select the computation source waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8, Math1-Math7).**
- Unit:** **Set the unit.**
- Label:** Math1. **Set the label.**
- Display:** OFF, ON. **Turns the waveform display on and off**

Configuring the FFT

Set the number of FFT points and window function. ► section 15.5

15.5 Performing User-Defined Computations


This section explains the following settings for performing user-defined computations.

- Computation
User definition (User Define), expression, unit, label, turning the waveform display on and off
- Scaling
- Computation start and end points
- FFT
- Filter
- Constant


► [Features Guide: “User-Defined Computation”](#)

MATH Menu

1. Press **MATH** to display the following menu.

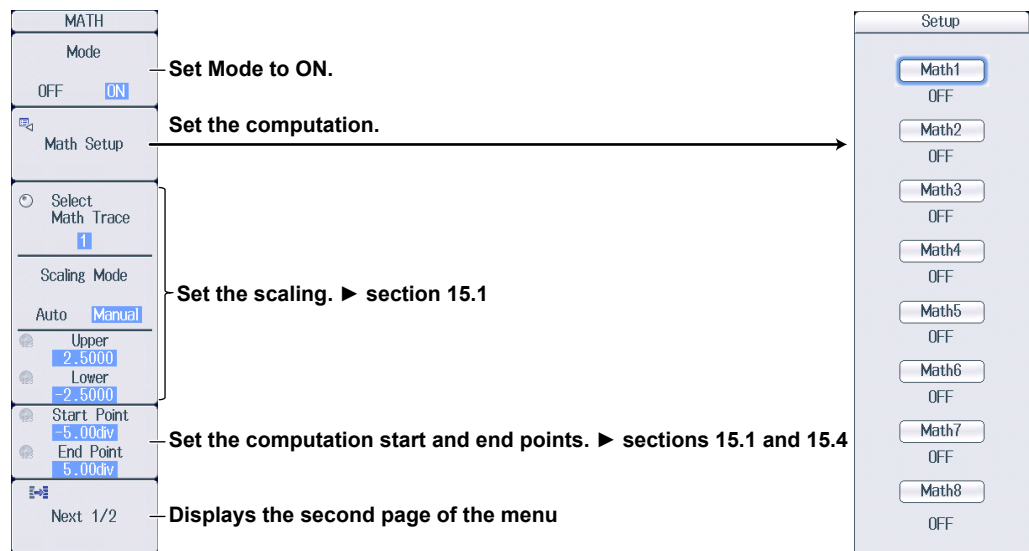


2. Press the **Next 1/2** soft key to display the 2/2 menu.

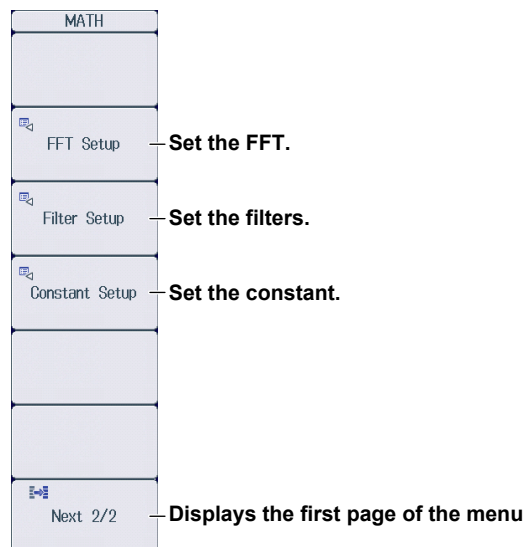

Configuring Computations (Math Setup)

1. Press the **Math Setup** soft key.
2. Press a soft key from **Math1** to **Math8** to display the following screen.

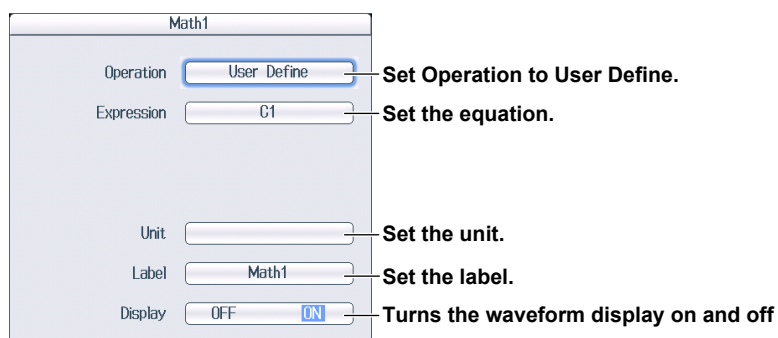


Setting the Expression (Expression)

3. Select **Expression** to display the following screen.

Add the results of automated measurement of waveform parameters to the expression.


Define an expression by combining computation source waveforms, operators, and functions.

Enter a character string from the history.

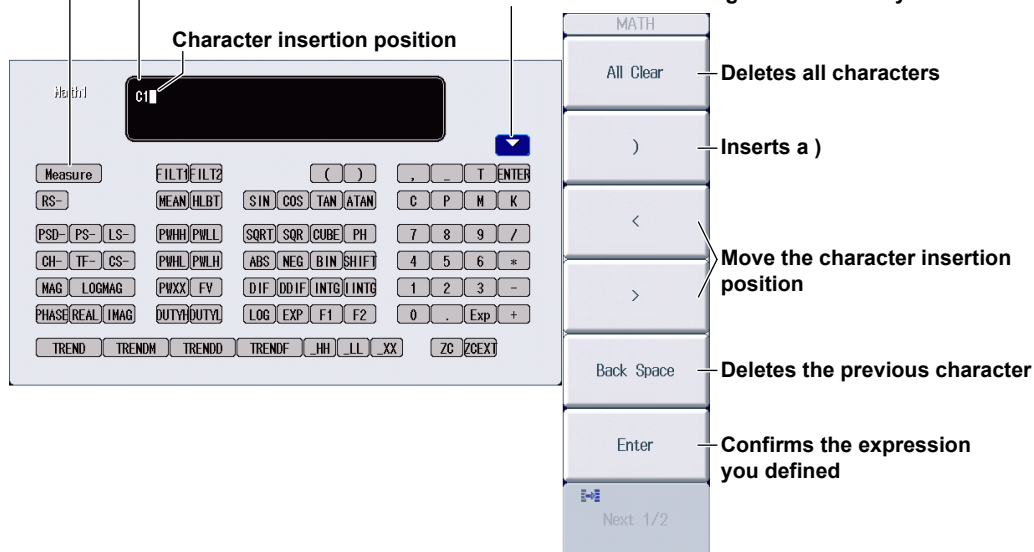


Configuring the FFT (FFT Setup)

Press the **FFT Setup** soft key to display the following screen.

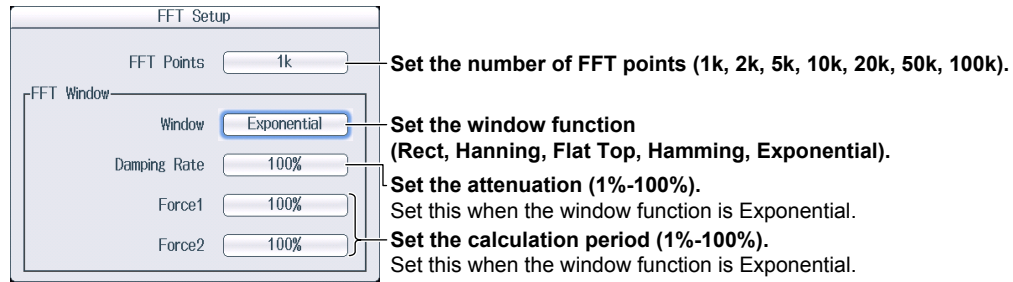

Configuring Filters (Filter Setup)


Press the **Filter Setup** soft key to display the following screen.

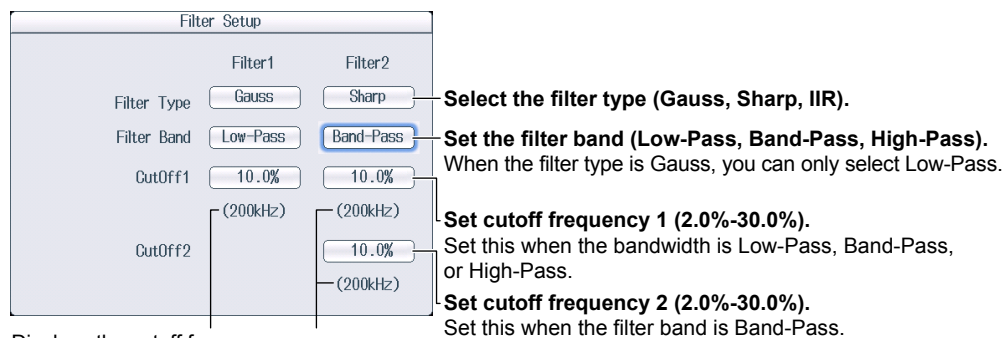

Displays the cutoff frequency as a percentage of the sample rate in use.

Defining Constants (Constant Setup)

Press the **Constant Setup** soft key to display the following screen.

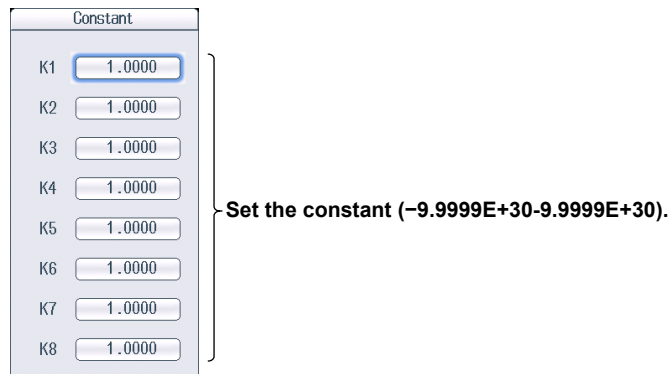

16.1 Displaying FFT Waveforms

This section explains the following settings for displaying power spectrum waveforms in the FFT window.

- FFT waveform display
- FFT
 - Spectrum type and sub type, analysis source waveform, window function
- Vertical scale
- Computation start point
- FFT points
- Main window's display ratio
- Window layout
- Horizontal axis
 - Scale, unit, zoom (display range)

► [Features Guide: “FFT”](#)

FFT Menu


1. Press **SHIFT+MATH** (FFT) to display the following menu.

FFT	
FFT1 OFF	FFT2 OFF
Display OFF ON	
FFT Setup	
Vert. Scale Mode Auto Manual	
Center 0.0000	Sensitivity 200.00E-03
Start Point -5.00div	
FFT Points 1k	
Next 1/2	

- Select whether to set FFT1 or FFT2.
- Turns the FFT display on and off
- Set the FFT.
- Set the vertical scaling mode (Auto, Manual).
- Set the vertical axis center and sensitivity.
 - Center ($-9.9999\text{E}+30$ to $9.9999\text{E}+30$)
 - Sensitivity ($1\text{E}-30$ to $1.9999\text{E}+30$)
- Set this when the vertical scale is Manual.
- Set the computation start point (-5div to -5div).
- The setting resolution varies depending on the display record length.
- Set the number of FFT points (1k, 2k, 5k, 10k, 20k, 50k, 100k).
- Displays the second page of the menu

16.1 Displaying FFT Waveforms

- Press the **Next 1/2** soft key to display the following menu.

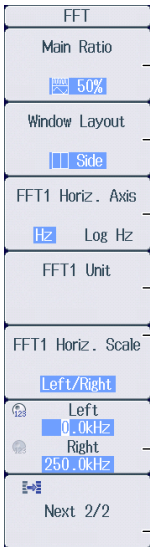

FFT

Main Ratio — Set the main window's display ratio (50%, 0%).

Window Layout — Set the window layout (Side, Vertical).

FFT1 Horiz. Axis Log Hz — Set the horizontal scale (Hz, Log Hz).

FFT1 Unit — Set the vertical scale unit.

FFT1 Horiz. Scale — Set the horizontal zoom mode (Auto, Left/Right, Center/Span).
Center/Span cannot be selected when the horizontal scale is set to Log Hz.


Left — Set the display range of the horizontal axis.

Right — When horizontal zoom is set to Left/Right

- Set the left and right edges (0Hz to maximum frequency).

The setting resolution varies depending on the number of FFT points.
The following relationship must be satisfied: (right edge – left edge) ≥ (10×setting resolution).

Next 2/2 — Displays the first page of the menu



Center — Set the display range of the horizontal axis.


Span — When horizontal zoom is set to Center/Span

- Set the center (0Hz to maximum frequency).
- Set the Span ((frequency resolution×10) to maximum frequency).

The setting resolution varies depending on the number of FFT points.

Configuring the FFT (FFT Setup)

Press the **FFT Setup** soft key to display the following screen.

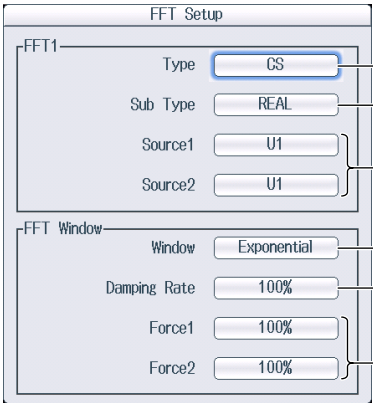

FFT Setup

FFT1

Type — Set the spectrum type (LS, RS, PS, PSD, CS, TF, or CH).

Sub Type — Set the spectrum sub type (REAL, IMAG, MAG, LOGMAG, PHASE).*

Source1 — Set the analysis source waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8, Math1-Math6).

Source2 — You can set Source 2 when the spectrum type is CS, TF, or CH.

FFT Window

Window — Set the window function (Rect, Hanning, Flat Top, Hamming, Exponential).

Damping Rate — Set the attenuation (1%-100%).

Force1 — Set this when the window function is Exponential.

Force2 — Set the calculation period (1%-100%).
Set this when the window function is Exponential.

* The available sub types vary depending on the spectrum type.

Type	Available Sub Types
LS, CS, TF	REAL, IMAG, MAG, LOGMAG, PHASE
RS, PS, PSD	MAG, LOGMAG
CH	MAG

17.1 Performing GO/NO-GO Determination with Waveform Zones


This section explains the following settings for performing GO/NO-GO determination with waveform zones:

- GO/NO-GO determination mode
- Editing the waveform zone
- Judgment condition
- Action
- Determination period

► [Features Guide: “Waveform Zone \(Wave Zone\)”](#)

GO/NO-GO Menu

Press **SHIFT+MEASURE** (GO/NO-GO) to display the following menu.

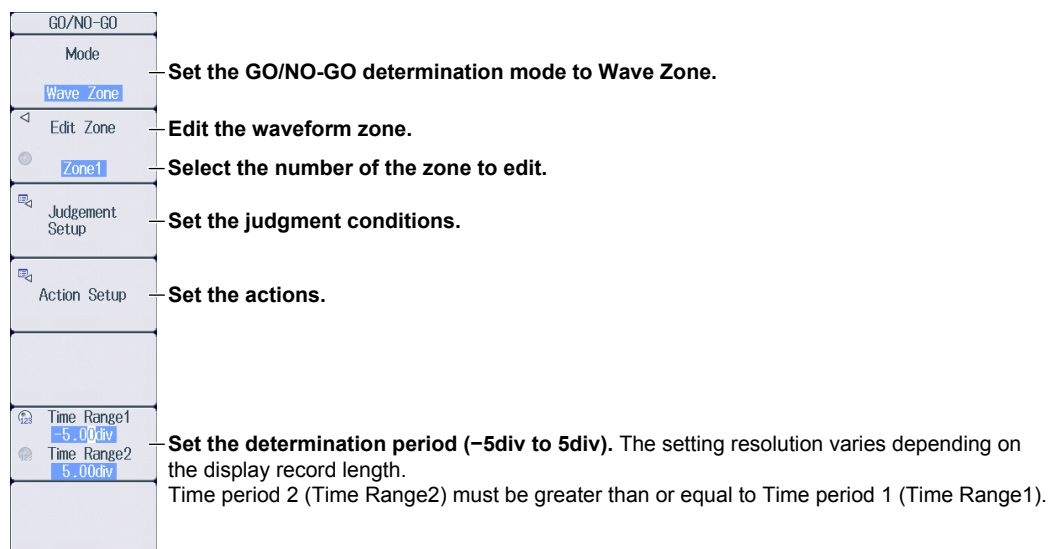

Editing Waveform Zones (Edit Zone)

1. Press the **Edit Zone** soft key described on the previous page to use the jog shuttle to adjust this setting.
If the jog shuttle is already controlling the Edit Zone soft key, proceed to step 2.
2. Use the **jog shuttle** to select the number of the zone that you want to edit (Zone1 to Zone6).
3. Press the **Edit Zone** soft key to display the following menu.

When in step 2, a zone number in which a created waveform zone does not exist is selected

Select the base waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8, Math1-Math8).

When you select the base waveform, the edit menu shown on the right appears.

When in step 2, a zone number in which a created waveform zone exists is selected

To clear the waveform zone that you are creating or have created and create a new waveform zone, select the base waveform on this menu.

Set the editing range (Whole, Part).

When the editing range is set to Whole

- Set the upper and lower limits (0.00div-10.00div).
- Set the left and right edges (0.00div-5.00div).

When the editing range is set to Part

- Set the time range (-5.00div to 5.00div).

Set the waveform zone save destination (Zone1-Zone6).

Saves the waveform zone

Setting the Judgment Conditions (Judgement Setup)

Press the **Judgement Setup** soft key to display the following screen.

You can set up to 16 conditions.

Set the judgment criterion (X, IN, OUT).

Set the source waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8, Math1-Math8).

Set the zone number (Zone1-Zone6).

#	Mode	Trace	Zone No.
1	X	U1	Zone1
2	X	U1	Zone1
3	X	U1	Zone1
4	X	U1	Zone1
5	X	U1	Zone1
6	X	U1	Zone1
7	X	U1	Zone1
8	X	U1	Zone1
9	X	U1	Zone1
10	X	U1	Zone1
11	X	U1	Zone1
12	X	U1	Zone1
13	X	U1	Zone1
14	X	U1	Zone1
15	X	U1	Zone1
16	X	U1	Zone1

Set the determination logic (AND, OR).

Set the action condition (Always, Fail, Success).

Set the sequence (Single, Continue).

Set the number of measurements (the number of waveform acquisitions) (Infinite, 1-65536).

Turns external start on and off

Setting Action Conditions (ActCondition)

Always: The action is always executed. The specified action, explained later, is executed each time a trigger occurs.

Fail: The action is executed when the GO conditions are not met.

Success: The action is executed when the GO conditions are met.

Setting the Sequence (Sequence)

Single: The action is executed once.

Continue: The action is executed repeatedly. It is repeated until the waveform is acquired the number of times specified by Acquisition Count. If Acquisition Count is set to Infinite, the action is repeated until waveform acquisition is stopped with the START/STOP key.

Setting Actions (Action Setup)

Press the **Action Setup** soft key to display the following screen.

Select the actions to execute (Beep, Print Image, Save Waveform, Save Numeric, Save Image).

The screenshot shows the 'Action Setup' dialog box. On the left, there is a list of actions with checkboxes: ☒ Beep, ☒ Print Image, ☒ Save Waveform, ☒ Save Numeric, and ☒ Save Image. The 'Save Image' checkbox is highlighted with a blue border. On the right, there are three sections for setting destinations:

- Save Waveform:** File Path (USB-0), Auto Naming (Numbering), File Name (empty), Data Type (Binary).
- Save Numeric:** File Path (USB-0), Auto Naming (Numbering), File Name (empty).
- Save Image:** File Path (USB-0), Auto Naming (Numbering), File Name (empty).

Callout boxes on the right provide additional instructions:

- Set the waveform data save destination.** ► section 22.3
Set this when Save Waveform is selected for the action.
- Set the numeric data save destination.** ► section 22.3
Set this when Save Numeric is selected for the action.
- Set the screen capture save destination.** ► section 22.3
Set this when Save Image is selected for the action.

17.2 Performing GO/NO-GO Determination with Waveform Parameters


This section explains the following settings for performing GO/NO-GO determination with waveform parameters.

- GO/NO-GO determination mode
- Judgment condition
- Action
- Determination period

► [Features Guide: “Waveform Parameters \(Parameter\)”](#)
“Automated Measurement of Waveform Parameters”

GO/NO-GO Menu

Press **SHIFT+MEASURE** (GO/NO-GO) to display the following menu.

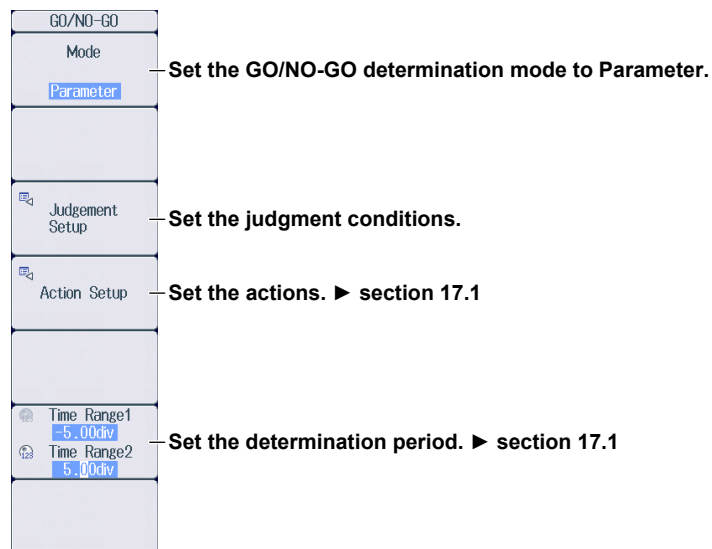

Setting the Judgment Conditions (Judgement Setup)

Press the **Judgement Setup** soft key to display the following screen.

You can set up to 16 conditions.

Set the judgment criterion (X, IN, OUT).

Set the source waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8, Math1-Math8).

Set the waveform parameters.

Judgement Setup					
#	Mode	Trace	Item	Upper	Lower
1	X	U1	Peak to Peak	0.0000	0.0000
2	X	U1	Peak to Peak	0.0000	0.0000
3	X	U1	Peak to Peak	0.0000	0.0000
4	X	U1	Peak to Peak	0.0000	0.0000
5	X	U1	Peak to Peak	0.0000	0.0000
6	X	U1	Peak to Peak	0.0000	0.0000
7	X	U1	Peak to Peak	0.0000	0.0000
8	X	U1	Peak to Peak	0.0000	0.0000
9	X	U1	Peak to Peak	0.0000	0.0000
10	X	U1	Peak to Peak	0.0000	0.0000
11	X	U1	Peak to Peak	0.0000	0.0000
12	X	U1	Peak to Peak	0.0000	0.0000
13	X	U1	Peak to Peak	0.0000	0.0000
14	X	U1	Peak to Peak	0.0000	0.0000
15	X	U1	Peak to Peak	0.0000	0.0000
16	X	U1	Peak to Peak	0.0000	0.0000

Logic: ☐ AND ☒ OR

ActCondition: ☐ Always ☒ Fail ☐ Success

Sequence: ☒ Single ☐ Continue

Acquisition Count:

Remote: ☒ OFF ☐ ON

Set the upper and lower limits of the parameters (-9.9999E+30 to 9.9999E+30).

Set the determination logic (AND, OR).

Set the action conditions. ► section 17.1

Set the sequence. ► section 17.1

Set the number of measurements (the number of waveform acquisitions) (Infinite, 1-65536).

Turns external start on and off

Setting Waveform Parameters (Item)

You can use all automatically measured waveform parameters as judgment conditions. Up to 16 parameters set as judgment conditions can be determined simultaneously. ► section 14.1

18.1 Setting Actions


This section explains the following settings for executing the action function.

- Action mode
- Action

► Features Guide: “Action”

ACTION Menu


Press **SHIFT+MODE** (ACTION) to display the following menu.

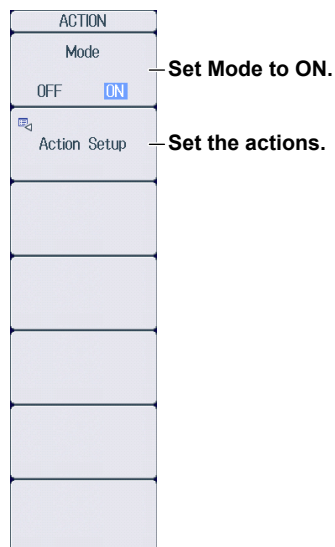

Setting Actions (Action Setup)

Press the **Action Setup** soft key to display the following screen.

Select the actions to execute (Beep, Print Image, Save Waveform, Save Numeric, Save Image).

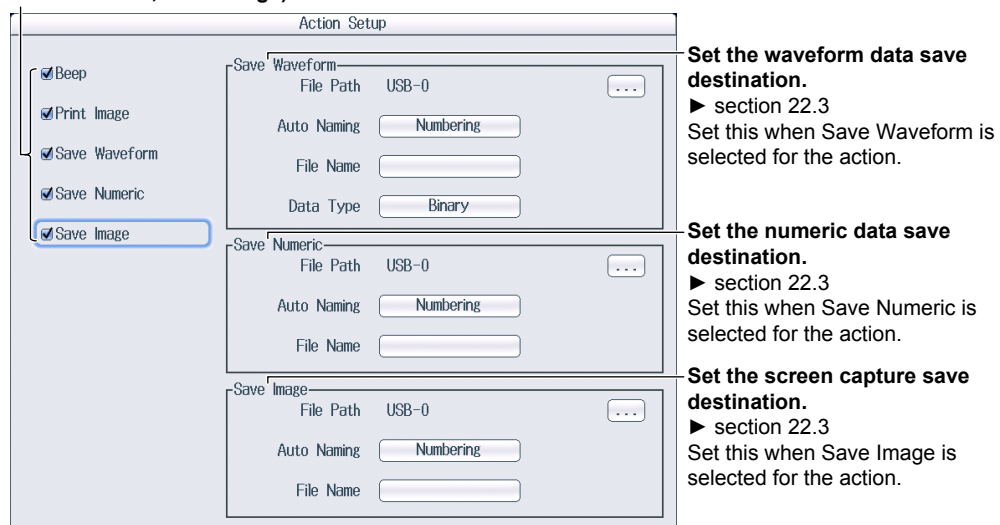

Executing Actions

Starting

1. Set the following functions, and press **START/STOP**. The actions are executed according to the settings.

An icon  appears in the top center of the screen when actions are being executed.

- Trigger ▶ chapter 3
- GO/NO-GO determination ▶ chapter 17

Stopping

2. Actions stop in the following conditions.
 - When the specified number of measurement count (waveform acquisition count) is reached
Measurement count (waveform acquisition count) ▶ section 4.1 or chapter 17
 - When waveform acquisition is stopped with the **START/STOP** key
When waveform acquisition is stopped with the **START/STOP** key, actions are executed once.

19.1 Searching for Edges


This section explains the following settings for searching for edges.

- Search type
- Search conditions
 - Source waveform, reference level to detect, edge polarity, hysteresis, and detection count
- Detected waveform display
- Detected point number
- Search start and end points
- Executing the search

► [Features Guide: “Edge Search \(Edge\)”](#)


SEARCH Edge Menu

Press **SHIFT+ZOOM** (SEARCH), the **Type** soft key, and then the **Edge** soft key to display the following menu.

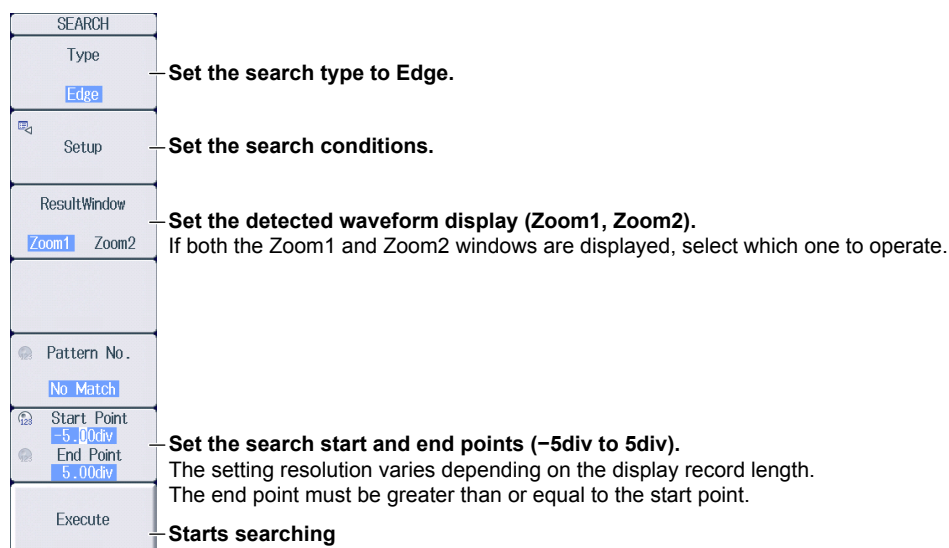

Setting Search Conditions (Setup)

Press the **Setup** soft key to display the following screen.

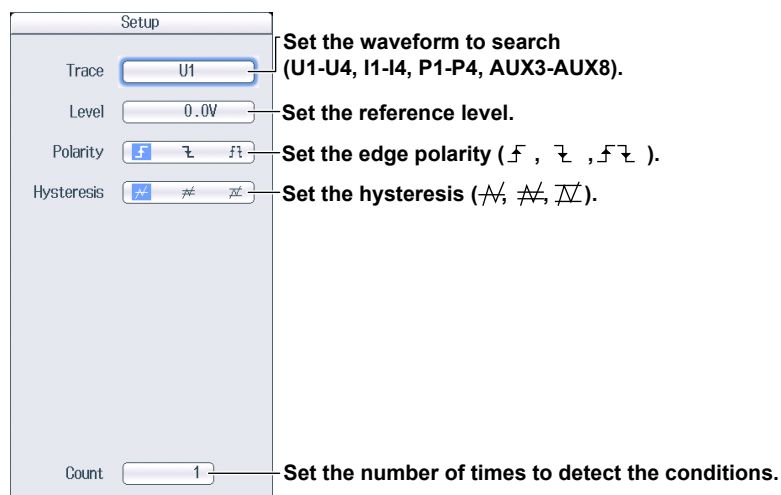

Setting the Detected Waveform Display (Result Window)

Press the **Result Window** soft key to select which zoom window displaying the search waveform to operate.


The search waveform that includes the search point specified by the detected point number (Pattern No.) described later is displayed in the zoom windows. If both the Zoom1 and Zoom2 windows are displayed, select which one to operate.

- If only one of the two zoom windows is displayed, you do not have to select the window.
- If both Zoom1 and Zoom2 are not displayed, Zoom1 will be displayed when you press SHIFT+ZOOM (SEARCH) to display the SEARCH menu.

Executing a Search (Execute)

Press the **Execute** soft key to execute the search.

If the PX8000 finds points that match the search conditions (detected points), it shows detected point numbers (0, 1, 2, etc.) from the left of the waveform display in the order that the points were detected.

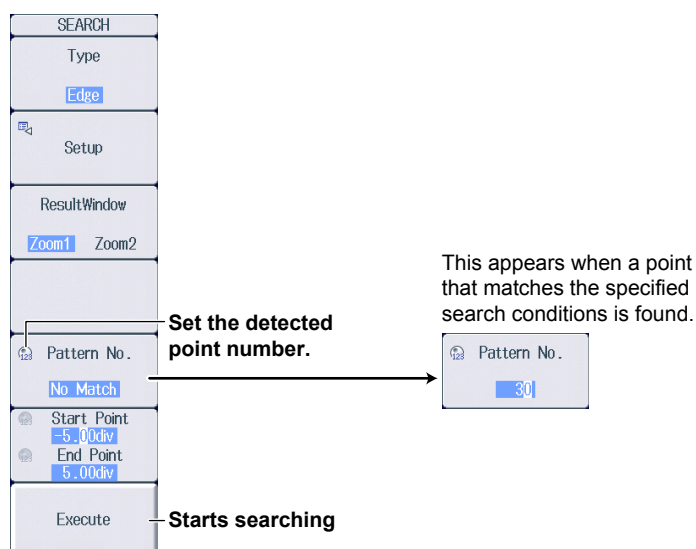

Setting the Detected Point Number

Set the detected point number. The detected waveform appears in the zoom window with the detected point corresponding to the specified detected point number at the center.

19.2 Searching for a Specific Time


This section explains the following settings for searching for a specific time.

- Search type
- Search conditions
Year, month, day, time
- Executing the search

► [Features Guide: “Time Search \(Time\)”](#)


SEARCH Time Menu

Press **SHIFT+ZOOM** (SEARCH), the **Type** soft key, and then the **Time** soft key to display the following menu.

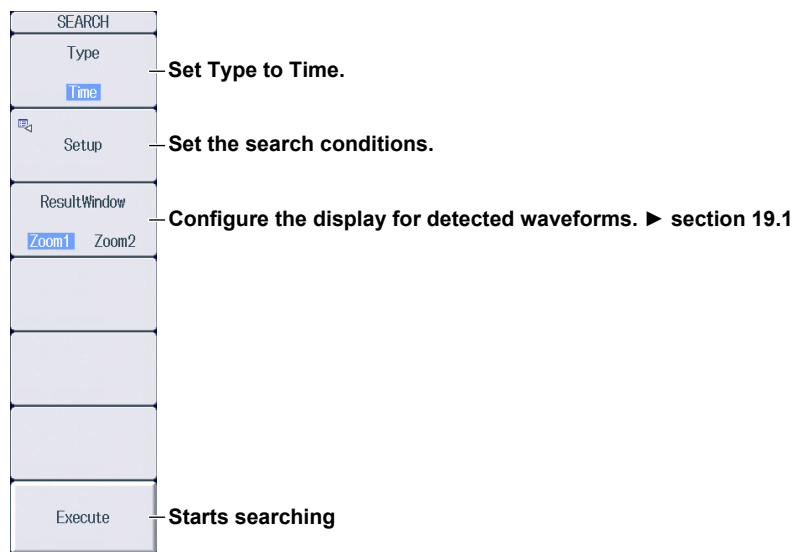

Setting Search Conditions (Setup)

Press the **Setup** soft key to display the following screen.

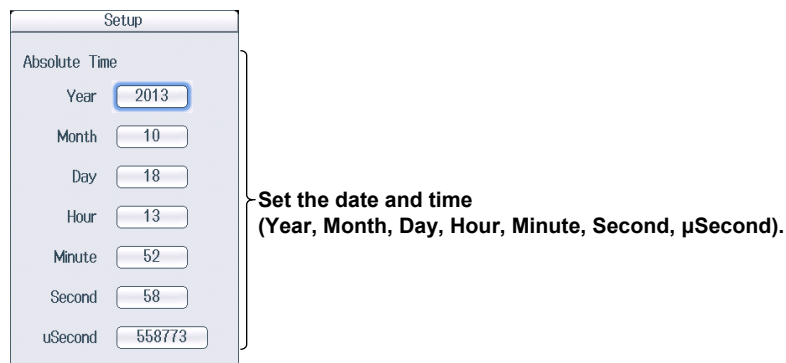

Executing a Search (Execute)

Press the **Execute** soft key to execute the search.

The detected waveform appears in the zoom window with the specified time at the center.

20.1 Displaying Waveform History Waveforms


This section explains the following settings for displaying history waveforms, which are waveforms that were previously saved to acquisition memory.

- Display mode
- Highlight display
- Display range
- List of history waveforms
- Clearing all the history waveforms

► **Features Guide: “Displaying and Searching History Waveforms”**

HISTORY Menu

Press **SHIFT+NUMERIC** (HISTORY) to display the following menu.

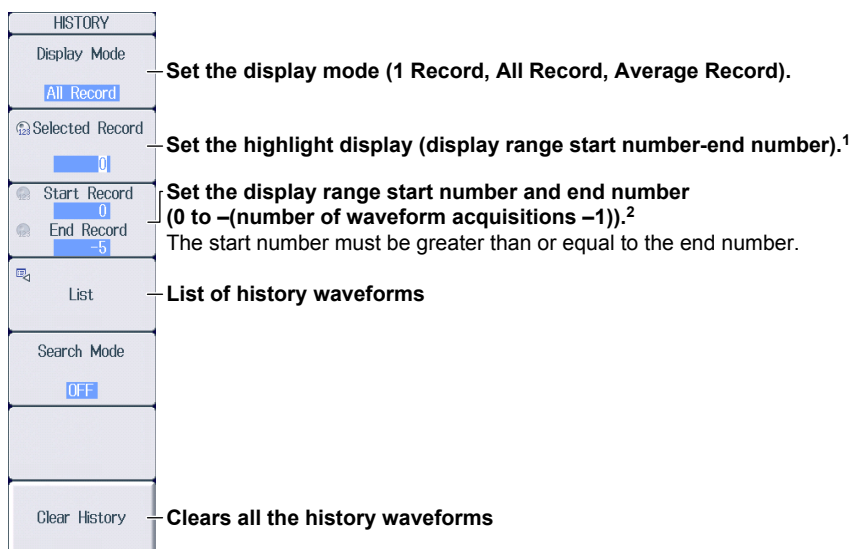

¹ This setting appears when Display Mode is set to 1 Record or All Record.

² The number of waveform acquisitions that can be specified is up to the number of history waveforms that can be held in the acquisition memory.

Setting the Display Mode (Display Mode)

1 Record: Only the waveform corresponding to the selected record number is displayed.¹

All Record: All selected waveforms are superimposed on each other.² All other waveforms¹ are displayed in the normal color.

Average Record: All selected waveforms² are linearly averaged and displayed.

¹ Waveforms specified by Selected Record for highlighting

² Waveforms in the display range specified by Start Record and End Record

Note

- After you execute a search on the history waveforms, the only waveforms that are displayed are those that meet the search conditions. To display all the history waveforms in acquisition memory again, turn the history waveform search feature off.
- The averaging feature requires a certain amount of acquisition memory. If this is not available, you will not be able to display the Average Record.

List of History Waveforms (List)

Press the **List** soft key to display the following screen.

Record number

Timestamp (time reference time information of each history waveform)

List

0000 12:50:25.572753

#-0001 12:50:25.254756

#-0002 12:50:24.894759

#-0003 12:50:24.576763

#-0004 12:50:24.258766


#-0005 12:50:23.940769

History waveform list

You can use the jog shuttle to scroll the list and specify the data to highlight.

Note

Notes on Using the History Feature

- You can start waveform acquisition when the HISTORY menu is displayed. However, you cannot change the history feature settings while waveform acquisition is in progress.
- When the acquisition mode is set to Average, you cannot use the history feature.
- If you stop waveform acquisition, even if one complete screen's worth of waveform data has not been acquired, the waveform at which the trigger occurred is displayed as a single history waveform.
- The settings are restricted so that the following relationship is retained: Last record (End Record) ≤ Selected Record ≤ first record (Start Record).
- When you load waveform data from the specified storage medium, history waveforms up to that point are cleared. The loaded waveform data is placed in record number zero. If you load a file containing multiple history waveforms, the latest waveform is placed in zero, and earlier waveforms are placed in order to record numbers -1, -2, and so on.
- Computation and automated measurement of waveform parameters are performed on the waveform of the record number specified by Selected Record. You can analyze old data as long as you do not overwrite the acquisition memory contents by restarting waveform acquisition. If Display Mode is set to Average Record, analysis is performed on the averaged waveform.
- If many history waveforms are selected, it may take a long time to display all waveforms or average waveforms. If this happens, the  icon appears at the top of the screen. To cancel the operation, set Display Mode to 1 Record.
- History waveforms are cleared when you turn the power off.

20.2 Searching History Waveforms

This section explains the following settings for searching history waveforms.

- Search mode
- Search conditions
Search zone, search parameters, search condition, source waveform, search window (upper and lower limits and left and right edges), search logic, and measurement time period of the parameters
- Executing the search

► **Features Guide: “Search Condition Settings for Zone Searching (Search Setup)”**
“Search Condition Settings for Waveform Parameter Searching (Search Setup)”

HISTORY Menu

Press **SHIFT+NUMERIC** (HISTORY) to display the following menu.

HISTORY	
Display Mode	
All Record	
Selected Record	
0	
Start Record	
0	
End Record	
-5	
List	
Search Mode	
OFF	
Clear History	

Set the search mode (OFF, Zone, Parameter).

Setting the Zone Search (Search Setup)

Press the **Search Mode** soft key, the **Zone** soft key, and then the **Search Setup** soft key to display the following menu.

Search Setup	
Select Zone	Select the search zone (Zone1-Zone4).
Zone1	
Condition	Set the search condition (OFF, IN, OUT).
OFF	
Source	Set the source waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8).
U1	
Upper	Set the upper and lower limits of the search window (-5.00div to 5.00div). The upper limit must be greater than or equal to the lower limit.
0.50div	
Lower	
-0.50div	
Left	Set the left edge and right edge of the search window (-5div to 5div). The setting resolution varies depending on the display record length.
-3.00div	
Right	The right edge must be greater than or equal to the left edge.
-2.50div	
Logic	Set the search logic (AND, OR).
AND	
Execute Search	

Proceed to executing the search on the next page.

Setting the Waveform Parameter Search (Search Setup)

1. Press the **Search Mode** soft key, the **Parameter** soft key, and then the **Search Setup** soft key to display the following menu.

Search Setup	
Select Param	Select the search parameter (Param1-Param4).
Param1	
Condition	Set the search condition (OFF, IN, OUT).
OFF	
Source	Set the waveform to search and parameters.
U1	
Upper	Set the upper and lower limits of the search condition (-9.9999E+30 to 9.9999E+30).
0.0000	
Lower	
0.0000	
Logic	Set the search logic (AND, OR).
AND	
Time Range1	Set the parameter measurement time period (-5div to 5div). The setting resolution varies depending on the display record length.
-5.00div	
Time Range2	Time period 2 (Time Range2) must be greater than or equal to Time period 1 (Time Range1). The maximum number of data points that are measured is 100 Mpoint from Time Range 1.
5.00div	
Execute Search	


Setting the Waveform to Search and the Parameter (Source)

2. Press the **Source** soft key to display the following menu.

Source	
Trace	Set the source waveform (U1-U4, I1-I4, P1-P4, AUX3-AUX8).
U1	
Item	Set the waveform parameter type. ► section 14.1
Peak to Peak	

Executing a Search (Execute Search)

After setting the search conditions, press **ESC** to return to the HISTORY menu.

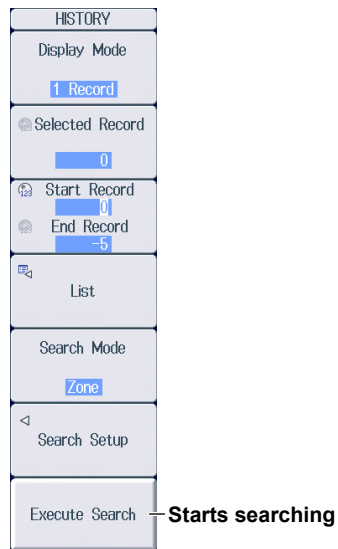

21.1 Loading Roll Paper Into the Built-In Printer (Optional)

This section explains how to load roll paper into the built-in printer (/B5 option).

Printer Roll Paper

Only use YOKOGAWA roll paper for the PX8000. When using the printer for the first time, use the roll paper supplied with the PX8000. When you need extra roll paper, please contact your nearest YOKOGAWA dealer.

Part Number: B9988AE

Specifications: Heat-sensitive paper, 10 m

Minimum Quantity: 10 rolls

Handling Roll Paper

The roll paper is made of heat-sensitive paper that changes color thermochemically. Please read the following information carefully.

Storage Precautions

The heat-sensitive paper changes color gradually at temperatures of approximately 70°C or higher. The paper can be affected by heat, humidity, or chemicals, whether something has been recorded on it or not. As such, please follow the guidelines listed below.

- Store the paper in a cool, dry, and dark place.
- Use the paper as quickly as possible after you break its protective seal.
- If you attach a plastic film that contains plasticizing material such as vinyl chloride film or cellophane tape to the paper for a long time, the recorded sections will fade due to the effect of the plasticizing material. Use a holder made of polypropylene to store the roll paper.
- When starching the record paper, do not use starches containing organic solvents such as alcohol or ether. Doing so will change the paper's color.
- We recommend that you make copies of the recordings if you intend to store them for a long period of time. Because of the nature of heat-sensitive paper, the recorded sections may fade.

Handling Precautions


- Only use genuine YOKOGAWA roll paper.
- If you touch the roll paper with sweaty hands, there is a chance that you will leave fingerprints on the paper or smudge the recorded sections.
- If you rub the surface of the roll paper against something hard, there is a chance that the paper will change color due to frictional heat.
- If the roll paper comes into contact with chemicals, oil, and the like, there is a chance that the paper will change color or that the recorded sections will disappear.


Loading the Roll Paper



CAUTION


- Do not touch the print head. If you do, you may burn yourself.
- Do not touch the roll paper cutter section at the end of the printer cover. Doing so may cause injury.

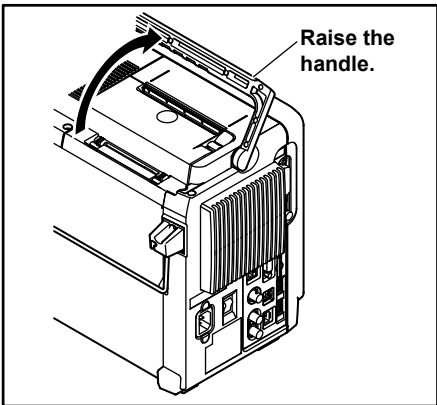- 

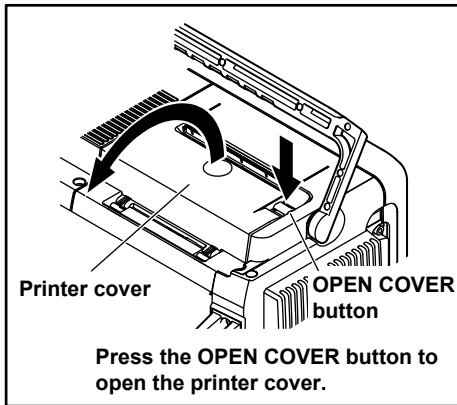Raise the handle.
- 


Printer cover

OPEN COVER button

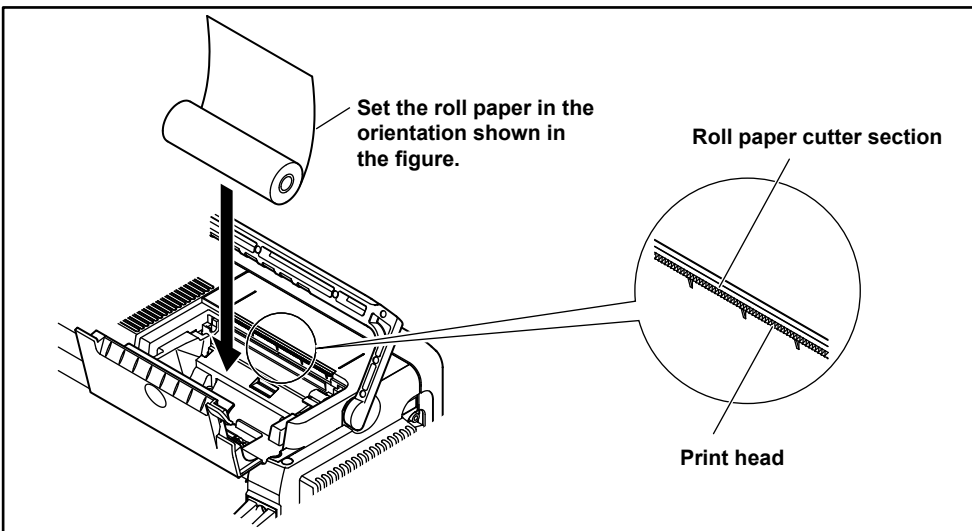
Press the OPEN COVER button to open the printer cover.
- 

Set the roll paper in the orientation shown in the figure.

Roll paper cutter section

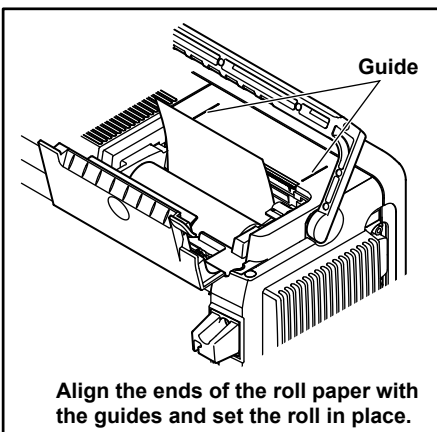Print head
- 

Guide

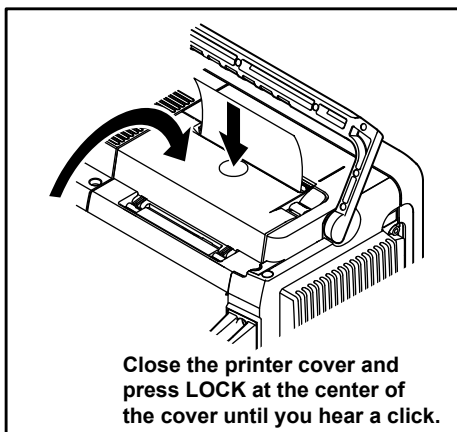Align the ends of the roll paper with the guides and set the roll in place.
- 

Close the printer cover and press LOCK at the center of the cover until you hear a click.

21.2 Printing on the Built-in Printer (Option)


This section explains the following settings for printing the image that is displayed on the PX8000 using the built-in printer (/B5 option).

- Print destination
- Comment

► [Features Guide: “Printing from the Built-In Printer \(BuiltIn; option\)”](#)

PRINT MENU Menu

Press **SHIFT+PRINT** (MENU), the **Print To** soft key, and then the **BuiltIn** soft key to display the following menu.

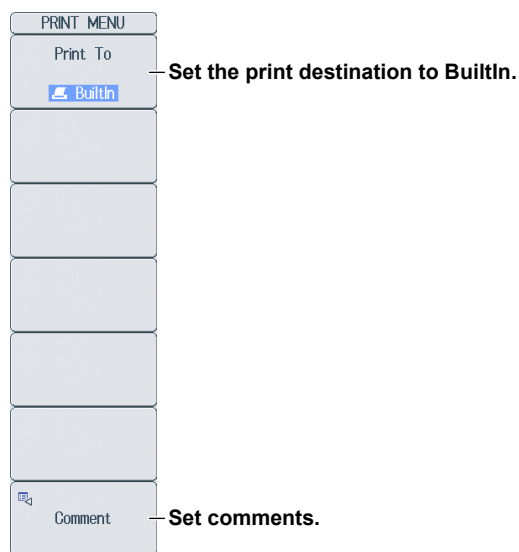

Starting to Print

Press **PRINT** to print the image that is displayed on the screen using the built-in printer.

21.3 Saving Screen Captures to Files

This section explains the following settings for saving screen captures to files.

- Print destination
- Data format
- Color
- Background transparency, frame on/off
- Save destination and file name


You can save screen captures from the PRINT MENU menu, SAVE menu, and FILE Others Save menu. The screen capture settings are shared among these menus.

This section describes how to save screen captures from the PRINT MENU menu and SAVE menu. For instructions on how to save from the FILE Others Save menu, see section 22.6.

► [Features Guide: “Saving Screen Captures \(File\)”](#)

PRINT MENU Menu

Press **SHIFT+PRINT** (MENU), the **Print To** soft key, and then the **File** soft key to display the following menu.

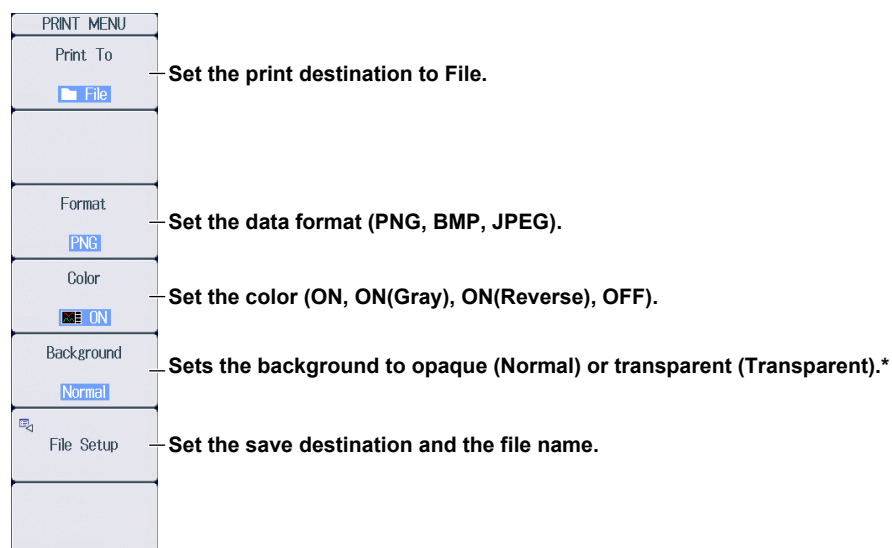

* This appears when the data format is set to PNG.
When the data format is set to JPEG, the frame on/off setting appears.

Setting the Save Destination and the File Name (File Setup)

Press the **File Setup** soft key to display the following screen.




Starting to Save

Press **PRINT** to save the screen capture file to the specified folder.

SAVE Menu


Press **SHIFT+SAVE** (MENU) to display the following menu.

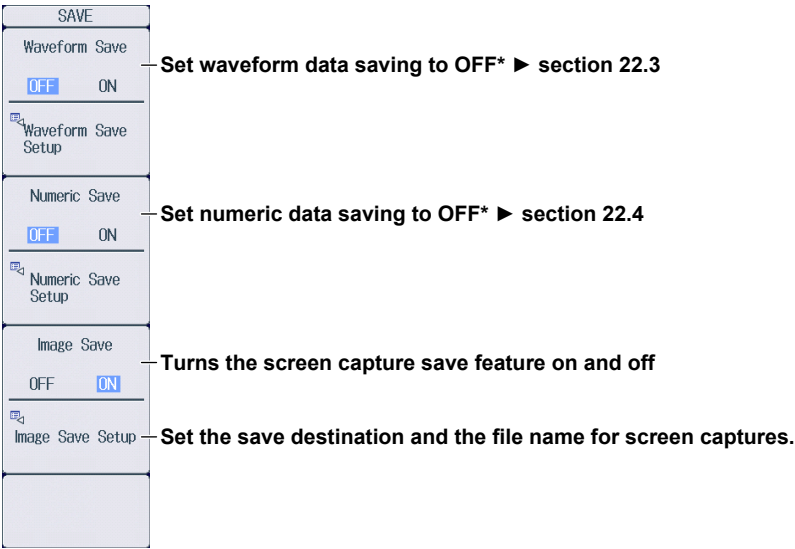

* If the saving of waveform data and numeric data is turned on, the corresponding data will also be saved according to the specified save destinations and file names. Here, the settings for saving only the screen capture are shown.

Setting the Save Destination and the File Name of the Screen Capture (Image Save Setup)

Press the **Image Save Setup** soft key to display the following screen.

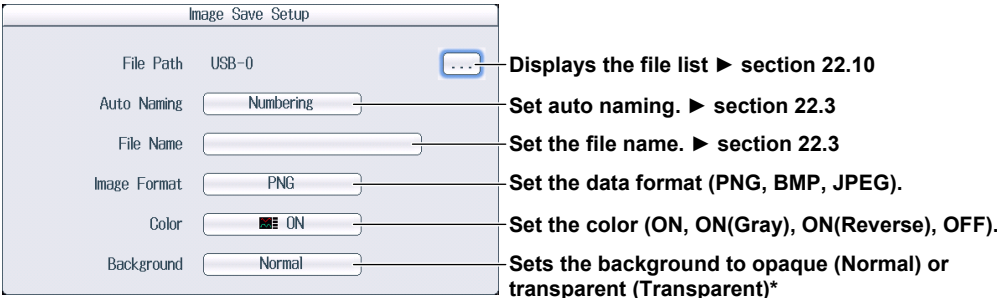

* This appears when the data format is set to PNG.
When the data format is set to JPEG, the frame on/off setting appears.

Starting to Save

Press **SAVE** to save the screen capture file to the specified folder.

22.1 Connecting Storage Media


This section explains how to connect the following types of storage media for saving and loading data from the PX8000.

- SD memory card
- USB storage device

SD Memory Card



CAUTION

- Do not insert the SD memory card in the wrong direction. Doing so may damage the SD memory card and the PX8000.
- Inserting and removing the SD memory card quickly (within the span of a second) may damage the PX8000.
- Removing the SD memory card from the PX8000 while the card is being accessed may corrupt the data on the SD memory card.
- An icon  appears at the top center of the screen when the SD memory card is being accessed.

SD Memory Cards That Can Be Used

You can use memory cards that conform to the SD or SDHC standard with the PX8000. For details, contact your nearest YOKOGAWA dealer.

Note


When using an SD memory card with a PC, make sure that the PC is compatible with the SD memory card. Also, depending on the type of PC, some of the SD cards listed above may not function properly. Make sure that the card that you intend to use is compatible with your PC.

How to Insert an SD Memory Card

Insert the SD memory card into the slot. The front of the card should be facing you.

The SD memory card slot is on the left side panel of the PX8000.


If you are using an SD memory card that has a write-protection feature and you want to save data to or format the card, disable the write-protection feature before you insert the SD memory card into the PX8000.

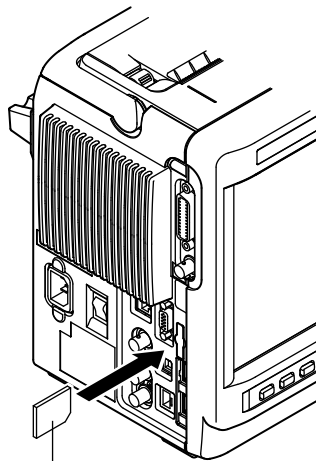

SD memory card

Removing the SD Memory Card

Push the SD memory card with your finger and release to eject the card.
Remove the SD memory card.

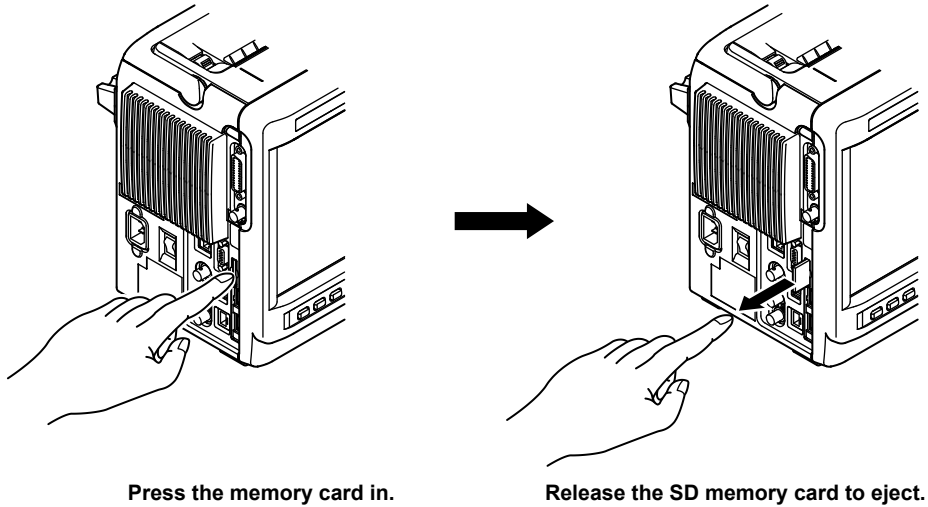


General SD Memory Card Handling Precautions

Follow the general handling precautions that are provided with your SD memory card.

USB Storage Device

CAUTION

- Do not remove the USB storage device or turn off the power when the device is being accessed. If you do so, the data on the USB storage device may be corrupted.
- An icon  appears at the top center of the screen when the USB storage device is being accessed.

Compatible USB Storage Devices

You can use USB storage devices that are compatible with USB Mass Storage Class version 1.1.


Note

- Only connect a USB keyboard, mouse, printer, or storage device to the USB connector for peripherals.
- The PX8000 can handle up to four storage devices. If the connected device is partitioned, the PX8000 treats each partition as a separate storage device.
- Connect USB storage device directly, not through a USB hub.
- Do not connect and disconnect the two USB devices repetitively. Provide a 10-second interval between removal and connection.

How to Connect a USB Storage Device

When connecting a USB storage device to the PX8000 USB port, connect the USB cable directly as shown in the figure below. You can connect/disconnect a USB cable at any time regardless of whether the PX8000 is on or off (hot-plugging is supported). Connect the type A connector of the USB cable to the PX8000, and connect the type B connector to the USB storage device. If you connect a USB storage device when the power switch is on, the device becomes available for use after the PX8000 identifies it.

The PX8000 has two USB ports: USB-0 and USB-1. The port numbers are not fixed. The port at which the first USB storage device is detected becomes USB-0. The second detected USB storage device becomes USB-1.

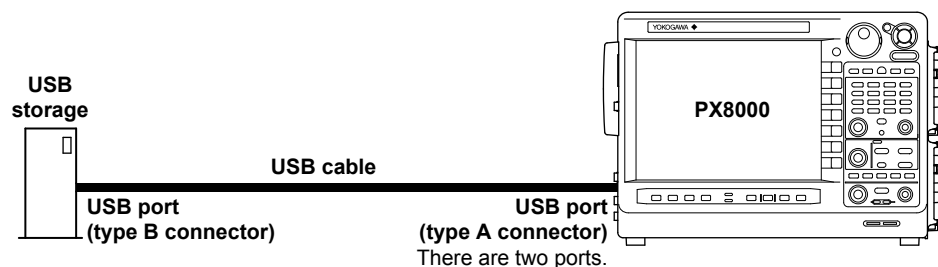

General USB Storage Device Handling Precautions

Follow the general handling precautions that are provided with your USB storage device.

22.2 Formatting Storage Media

This section explains how to format storage media.

Storage management


- Selecting the storage medium to format
- Executing the format

CAUTION

- When you format a storage medium, all the data on it is deleted.
- If a formatted storage medium cannot be detected by the PX8000, use the PX8000 to format the storage medium again.


UTILITY System Config Menu

Press **UTILITY** and then the **System Config** soft key to display the following menu.

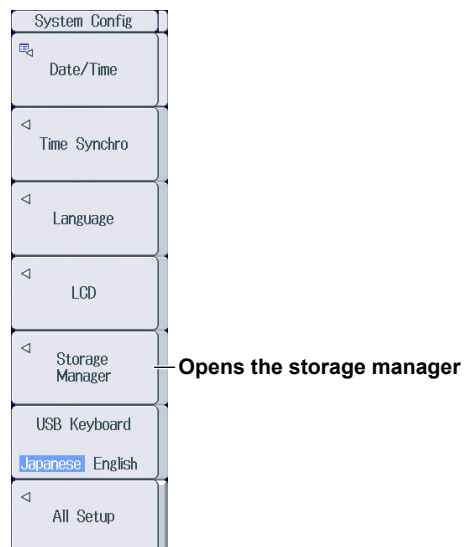

Setting Storage Management (Storage Manager)

Press the **Storage Manager** soft key to display the following menu.

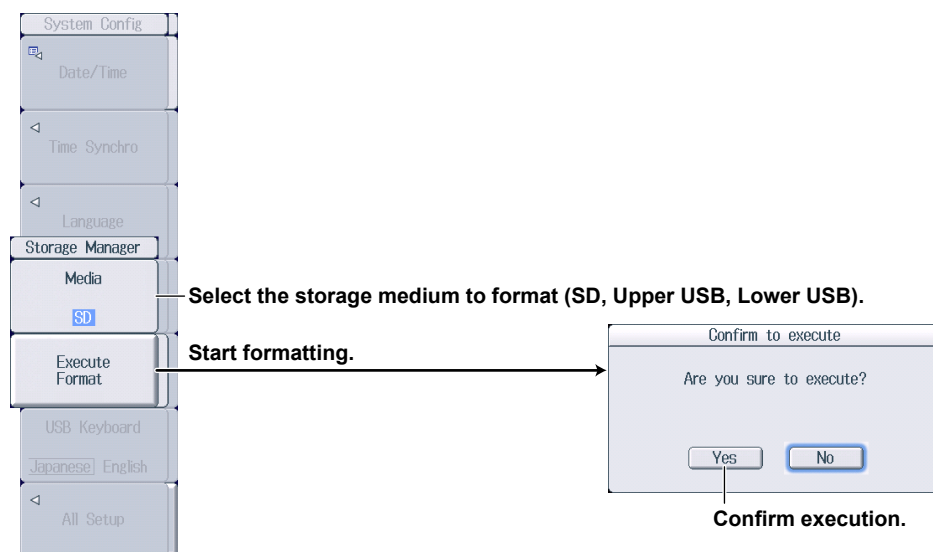

Storage Medium to Format (Media)

SD: SD memory card

Upper USB: The USB storage device that is connected to the PX8000's upper USB port (type A) for connecting peripheral devices.

Lower USB: The USB storage device that is connected to the PX8000's lower USB port (type A) for connecting peripheral devices.

22.3 Saving Waveform Data

This section explains the following settings for saving waveform data.


- Save destination
Drive (medium), folder
- File name
Auto naming, file name, comment
- Data type
- Save range
- Save conditions
Waveforms to save, history data range of waveforms to be saved, data removal interval, etc.
- Starting to Save

You can save waveform data from the FILE Waveform Save menu and SAVE menu. The settings for saving waveform data are shared among these menus.

► [Features Guide: “Saving Waveform Data \(Waveform\)”](#)

FILE Waveform Save Menu

Press **FILE** and then the **Waveform** soft key next to Save to display the following menu.

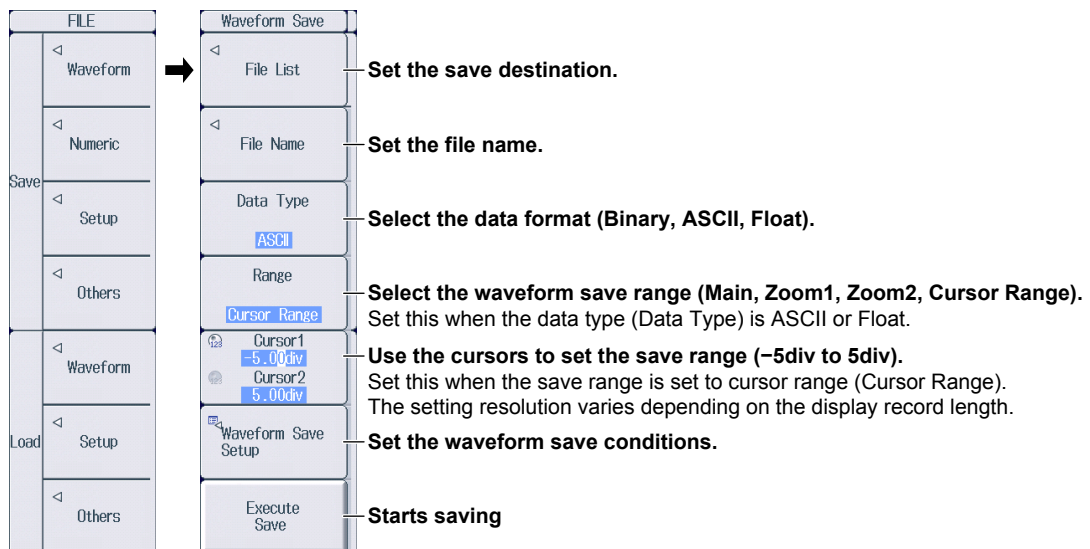

Selecting the Data Type (Data Type)

Binary:

The sampled data stored in the acquisition memory is saved to a file in binary format. The extension is .WPF. You can load this type of data into the PX8000.

ASCII:

The sampled data stored in the acquisition memory is converted using the specified range and saved to a file in ASCII format. The extension is .CSV. To save the data for MATLAB (numeric analysis software), the extension is .TXT. You cannot load either of these types of data into the PX8000.

Float:

The sampled data stored in the acquisition memory is converted using the specified range and saved to a file in 32-bit IEEE floating format. The extension is .FLD. You cannot load this type of data into the PX8000. If the file size would exceed 2 GB to create the file, it cannot be saved.


Selecting the Waveform Save Range (Range)

- Main: The range of data displayed in the main window is saved.
 Zoom1: The range data displayed in the Zoom1 window is saved.
 Zoom2: The range of data displayed in the Zoom2 window is saved.
 Cursor Range: The range of data specified by Cursor1 and Cursor2 is saved.

Setting the Save Destination (File List)

Press the **File List** soft key to display the following screen.

Operation menu ► section 22.10

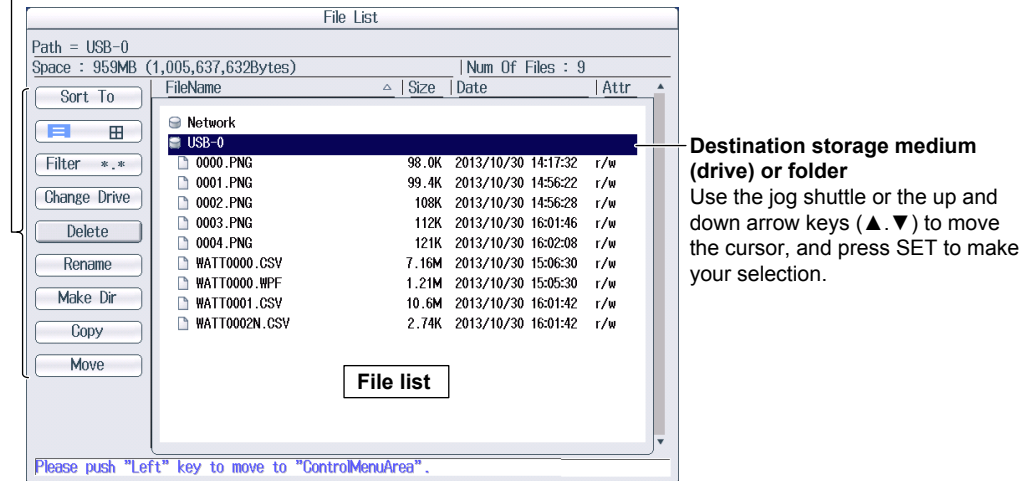


Note

You can also set the save destination drive by using the Change Drive item on the operations menu.


Save Destination (Save Path) Display Box

The save destination box appears at the bottom of the screen when the FILE Save menu is displayed. This box displays the file save destination, file name, and so on.

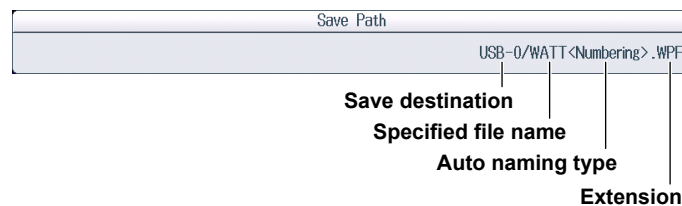


Assigning File Names (File Name)

Press the **File Name** soft key to display the following menu.

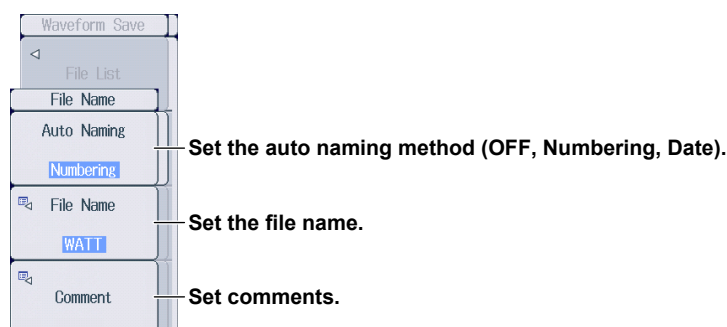

Setting Auto Naming (Auto Naming)

- OFF:** The auto naming feature is disabled. The name that you specify using the File Name setting is used. If there is a file with the same name in the save destination folder, you cannot save the data.
- Numbering:** The PX8000 automatically adds a four-digit number between 0000 to 9999 after the common name specified using the File Name setting (up to four characters) when it saves files.
- Date:** The file name is the date and time (down to ms) when the file is saved. The file name specified for the File Name setting is ignored.

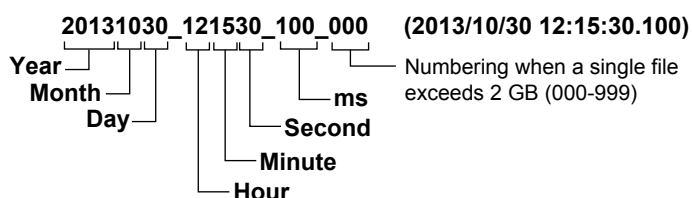

Regardless of whether the auto naming feature is set to OFF, Numbering, or Date, if the data size of a single file exceeds 2 GB, an underscore and a three-digit sequence number (000 to 999) is appended to the file name. The sequence number is incremented by one each time a file is added. This is appended only if the file exceeds 2 GB.

Setting the Comment (Comment)

You can add a comment that consists of up to 120 characters when you save a file. You do not have to enter a comment. All characters, including spaces, can be used in comments.

Setting the Waveform Save Conditions (Waveform Save Setup)

Press the **Waveform Save Setup** soft key to display the following screen.

History data range of the waveforms to be saved (One, All)

Select the waveforms that you want to save.

Select All ON.
All displayed waveforms are saved regardless of whether the individual waveforms in the table below are selected.

Math1 to Math8
Set these when Data Type is set to ASCII or Float. These do not appear for Binary.

Select Save Trace	
<input type="checkbox"/> All ON	
<input checked="" type="checkbox"/> U1	<input checked="" type="checkbox"/> AUX8
<input checked="" type="checkbox"/> I1	
<input checked="" type="checkbox"/> P1	<input checked="" type="checkbox"/> Math1
<input checked="" type="checkbox"/> U2	<input checked="" type="checkbox"/> Math2
<input checked="" type="checkbox"/> I2	<input checked="" type="checkbox"/> Math3
<input checked="" type="checkbox"/> P2	<input checked="" type="checkbox"/> Math4
<input checked="" type="checkbox"/> U3	<input checked="" type="checkbox"/> Math5
<input checked="" type="checkbox"/> I3	<input checked="" type="checkbox"/> Math6
<input checked="" type="checkbox"/> P3	<input checked="" type="checkbox"/> Math7
<input checked="" type="checkbox"/> AUX7	<input checked="" type="checkbox"/> Math8

Set these when Data Type is set to ASCII.

Interval (data removal interval)

OFF, Per5, Per10, Per20, Per50, Per100, Per200, Per500, Per1000, Per2000, Per5000

Time Info. (whether to save time information)

OFF, ON

Extension (file name extension)

csv, MATLAB*

Decimal Point (decimal point)

Point, Comma

* If MATLAB is selected, the extension will be set to .TXT.

History Data Range of Waveforms to Be Saved (History)

One: The one waveform that is specified with Selected Record on the HISTORY menu will be saved. To save an averaged history waveform, set the history feature's display mode to Average Record, and then select One.

All: All history waveforms within the range bounded by Start Record and End Record on the HISTORY menu will be saved. If you search for history waveforms, and then select All, only the detected waveforms will be saved.

Selecting the Waveforms to Save (Select Save Trace)

You can select All ON, U1 to U4, I1 to I4, P1 to P4, AUX3 to AUX8, and Math1 to Math8 waveforms. The displayed waveforms that you select are saved. The setup data for the saved waveforms are also saved.


- Waveforms that are not displayed will not be saved even if you select them.
- Math1 to Math8 are available when the data type (Data Type) is ASCII or Float.
 - If the computation mode on the MATH menu is set to OFF, Math1 to Math8 cannot be selected.
 - Any computation channels (Math1 to Math8) whose operation is set to OFF on the MATH menu cannot be selected.
 - Any computation channels (Math1 to Math8) whose display is set to OFF on the MATH menu will not be displayed. Therefore, they will not be saved.
- If the data type is set to Binary, source waveforms for waveform computation on the MATH menu are saved even if they are not displayed. Therefore, even though Math1 to Math8 are cannot be specified to be saved when the data type is set to Binary, when binary data is loaded, Math1 to Math8 may appear depending on the setup data of the MATH menu.
- If the data type is set to ASCII or Float and you select All for saving history waveforms, Math1 to Math8 will not be saved. If you want to save Math1 to Math8, set History to One.

Starting to Save (Execute Save)

Press the **Execute Save** soft key to save the waveform data file to the specified folder.


SAVE Menu

Press **SHIFT+SAVE** (MENU) to display the following menu.

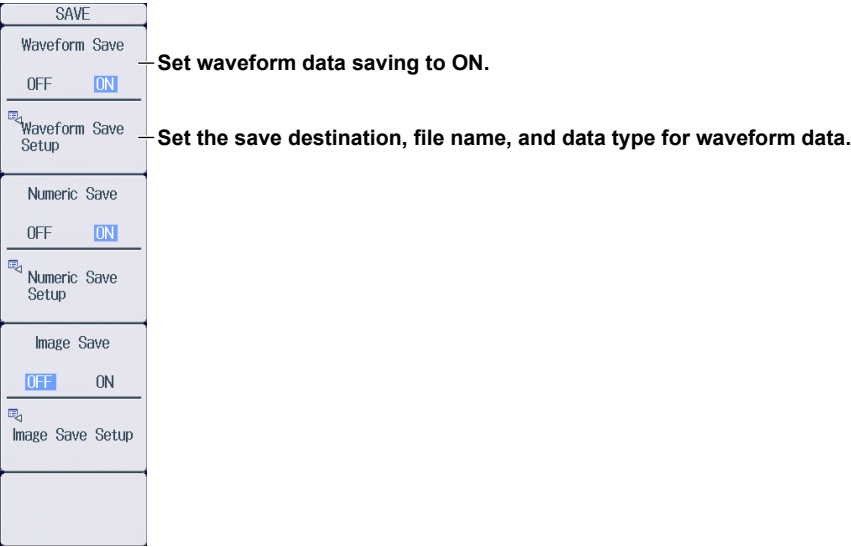

Setting the Save Destination, File Name, and Data Type for Waveform Data (Data Save Setup)

Press the **Waveform Save Setup** soft key to display the following screen.

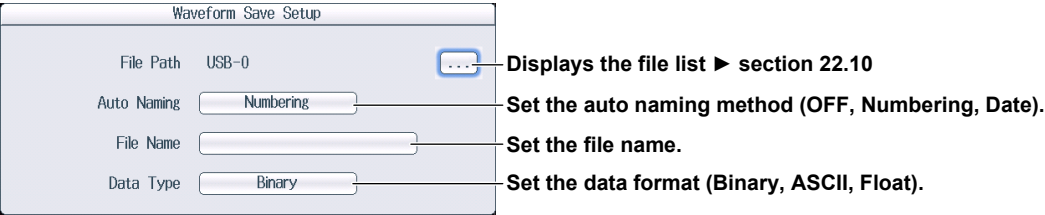

Starting to Save

Press **SAVE** to save the waveform data file to the specified folder.

If Numeric Save or Image Save on the SAVE menu is set to ON, the numeric data or screen capture data will also be saved.

Save Destination for Action Execution

In the specified drive, a folder is automatically created with the date (year, month, and day) as its name, and data is saved to files in that folder using names that are specified by the auto naming feature.

If the number of files in the save destination folder exceeds 1000, a new folder is automatically created with the date and an incremented sequence number (000 to 999) as its name, and the data continues to be saved in the new folder.

22.4 Saving Numeric Data

This section explains the following settings for saving numeric data.


- Save destination
- File name
- Data to save
- Decimal point
- Starting to Save

You can save numeric data from the FILE Numeric Save menu and SAVE menu. The settings for saving numeric data are shared among these menus.

► [Features Guide “Saving Numeric Data \(Numeric\)”](#)


FILE Numeric Save Menu

Press **FILE** and then the **Numeric** soft key next to Save to display the following menu.

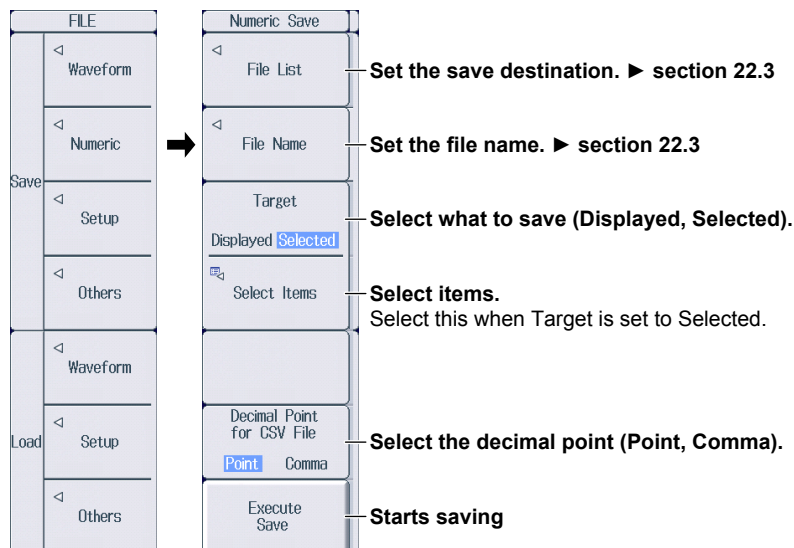

Save Destination (Save Path) Display Box

The save destination box appears at the bottom of the screen when the FILE Save menu is displayed. This box displays the file save destination, file name, and so on.

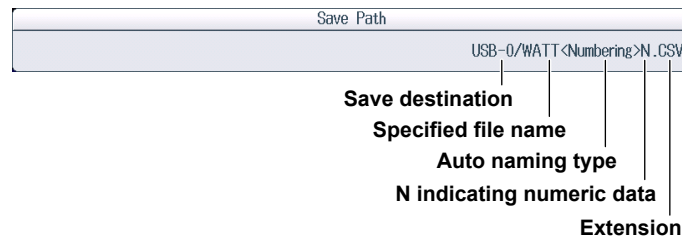

Selecting an Item

Press the **Select Items** soft key to display the following screen.

Selects all the numeric data items

Clears the selection of all the numeric data items

Selects the preset numeric data items

Items Settings							
Preset	All ON	All OFF	Preset				
Element	<input checked="" type="checkbox"/> Element1	<input checked="" type="checkbox"/> Element2	<input checked="" type="checkbox"/> Element3				
Function	<input type="checkbox"/> Σ A						
	<input checked="" type="checkbox"/> Urms	<input type="checkbox"/> Umn	<input type="checkbox"/> Udc	<input type="checkbox"/> Urnn	<input type="checkbox"/> Uac	<input checked="" type="checkbox"/> FreqU	<input type="checkbox"/> CRU
	<input checked="" type="checkbox"/> Irms	<input type="checkbox"/> Imn	<input type="checkbox"/> Idc	<input type="checkbox"/> Irnn	<input type="checkbox"/> Iac	<input checked="" type="checkbox"/> FreqI	<input type="checkbox"/> CIR
	<input checked="" type="checkbox"/> P	<input checked="" type="checkbox"/> S	<input checked="" type="checkbox"/> Q	<input checked="" type="checkbox"/> λ	<input checked="" type="checkbox"/> ϕ	<input type="checkbox"/> Pc	
	<input type="checkbox"/> U+peak	<input type="checkbox"/> U-peak	<input type="checkbox"/> I+peak	<input type="checkbox"/> I-peak	<input type="checkbox"/> P+peak	<input type="checkbox"/> P-peak	
	<input type="checkbox"/> η1	<input type="checkbox"/> η2	<input type="checkbox"/> η3	<input type="checkbox"/> η4			
	<input type="checkbox"/> F1	<input type="checkbox"/> F2	<input type="checkbox"/> F3	<input type="checkbox"/> F4	<input type="checkbox"/> F5	<input type="checkbox"/> F6	<input type="checkbox"/> F7
	<input type="checkbox"/> F8	<input type="checkbox"/> F9	<input type="checkbox"/> F10	<input type="checkbox"/> F11	<input type="checkbox"/> F12	<input type="checkbox"/> F13	<input type="checkbox"/> F14
	<input type="checkbox"/> F15	<input type="checkbox"/> F16	<input type="checkbox"/> F17	<input type="checkbox"/> F18	<input type="checkbox"/> F19	<input type="checkbox"/> F20	
	<input type="checkbox"/> FreqPLL1						
	<input type="checkbox"/> U(k)	<input type="checkbox"/> I(k)	<input type="checkbox"/> P(k)	<input type="checkbox"/> S(k)	<input type="checkbox"/> Q(k)	<input type="checkbox"/> λ(k)	<input type="checkbox"/> ϕ(k)
	<input type="checkbox"/> ϕU(k)	<input type="checkbox"/> ϕI(k)	<input type="checkbox"/> Z(k)	<input type="checkbox"/> Rs(k)	<input type="checkbox"/> Xs(k)	<input type="checkbox"/> Rp(k)	<input type="checkbox"/> Xp(k)
	<input type="checkbox"/> Uthd	<input type="checkbox"/> Ithd	<input type="checkbox"/> Pthd	<input type="checkbox"/> Uhdff(k)	<input type="checkbox"/> Ihdff(k)	<input type="checkbox"/> Phdff(k)	
	<input type="checkbox"/> Uthf	<input type="checkbox"/> Ithf	<input type="checkbox"/> Utif	<input type="checkbox"/> Itif	<input type="checkbox"/> hvf	<input type="checkbox"/> hcf	<input type="checkbox"/> K-factor
	<input type="checkbox"/> ϕU-Uj	<input type="checkbox"/> ϕU-Uk	<input type="checkbox"/> ϕU-li	<input type="checkbox"/> ϕUj-lj	<input type="checkbox"/> ϕUk-lk		
	<input type="checkbox"/> ϕI-lj	<input type="checkbox"/> ϕI-lk	<input type="checkbox"/> ϕI-lk				
	<input type="checkbox"/> ΔU1	<input type="checkbox"/> ΔU2	<input type="checkbox"/> ΔU3	<input type="checkbox"/> ΔUΣ	<input type="checkbox"/> ΔI		
	<input type="checkbox"/> ΔP1	<input type="checkbox"/> ΔP2	<input type="checkbox"/> ΔP3	<input type="checkbox"/> ΔPΣ			
	<input type="checkbox"/> AUX7	<input type="checkbox"/> AUX8	<input type="checkbox"/> Pm4				

Select the numeric items that you want to save.

Starting to Save (Execute Save)

Press the **Execute Save** soft key to save the numeric data file to the specified folder.

SAVE Menu

Press **SHIFT+SAVE** (MENU) to display the following menu.

SAVE

Waveform Save

OFF ON

Waveform Save Setup

Numeric Save

OFF ON

Numeric Save Setup

Image Save

OFF ON


Image Save Setup

Set numeric data saving to ON.

Set the save destination, file name, and data to save for numeric data.

Setting the Save Destination, File Name, and Data to Save for Numeric Data (Data Save Setup)

Press the **Numeric Save Setup** soft key to display the following screen.

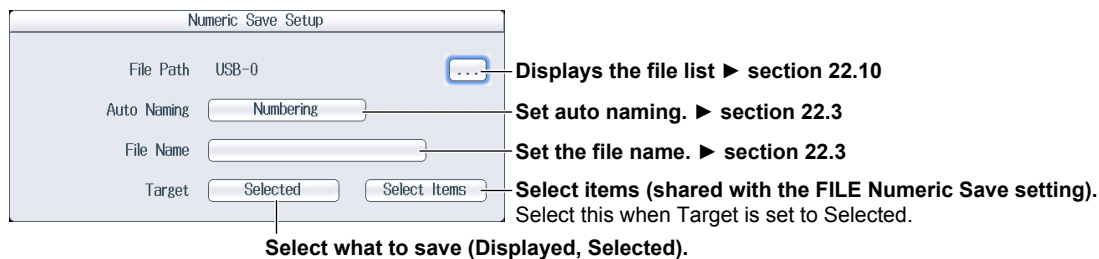

Starting to Save

Press **SAVE** to save the numeric data file to the specified folder.

If Waveform Save or Image Save on the SAVE menu is set to ON, the waveform data or screen capture data will also be saved.


22.5 Saving Setup Data

- This section explains the following settings for saving setup data. You can save setup data to a file.
- Save destination
 - File name
 - Starting to Save

► [Features Guide: “Saving Setup Data \(setup\)”](#)


FILE Setup Save Menu

Press **FILE** and then the **Setup** soft key next to Save to display the following menu.

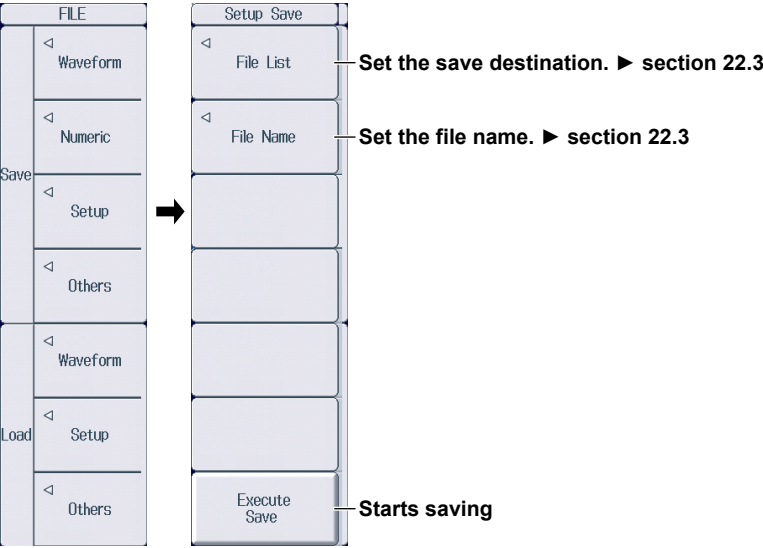

Save Destination (Save Path) Display Box

The save destination box appears at the bottom of the screen when the FILE Save menu is displayed. This box displays the file save destination, file name, and so on.

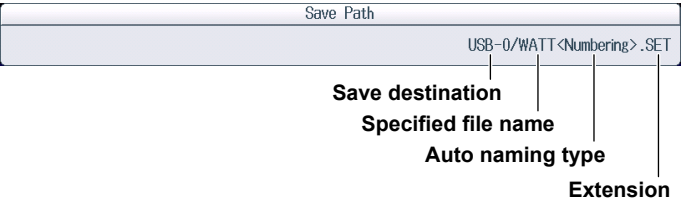

Starting to Save (Execute Save)

Press the **Execute Save** soft key to save the setup data file to the specified folder.

22.6 Saving Other Types of Data

This section explains the following settings for saving screen captures, snapshot waveforms, results of automated measurement of waveform parameters, and results of FFT.

- Save destination
- File name
- Data type to save
- Data format (for screen captures)
- Color (for screen captures)
- Starting to Save


You can save screen captures from the FILE Others Save, PRINT MENU menu, and SAVE menu. The screen capture settings are shared among these menus.

This section describes how to save screen captures from the FILE Others Save menu. For instructions on how to save from the PRINT MENU menu and SAVE menu, see section 21.3.

► **Features Guide: “Saving Other Types of Data (Others)”**


FILE Others Save Menu

Press **FILE** and then the **Others** soft key next to Save to display the following menu.

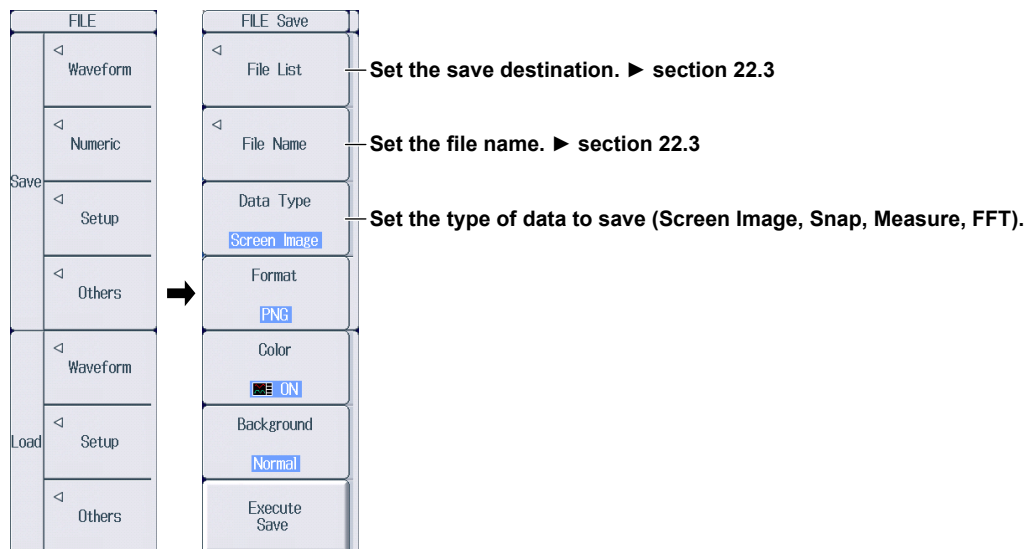

Save Destination (Save Path) Display Box

The save destination box appears at the bottom of the screen when the FILE Save menu is displayed. This box displays the file save destination, file name, and so on.

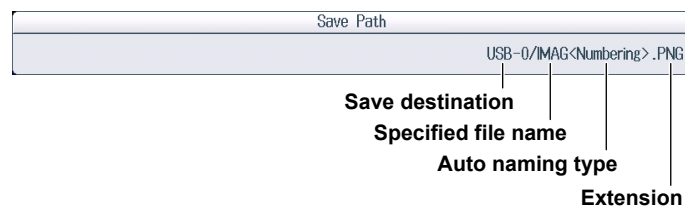

Setting the Data Type to Save (Data Type)

1. Press the **Data Type** soft key.

2. Set the type of data to save.


Screen Image: The displayed screen image is saved to a PNG, BMP, or JPEG file.

Snap: Waveform data captured in a snapshot is saved to an .SNP file.

Measure: The results of automated measurement of waveform parameters are saved to a CSV file.

FFT: The FFT analysis results are saved to a CSV file.

When Data Type Is Set to Screen Image

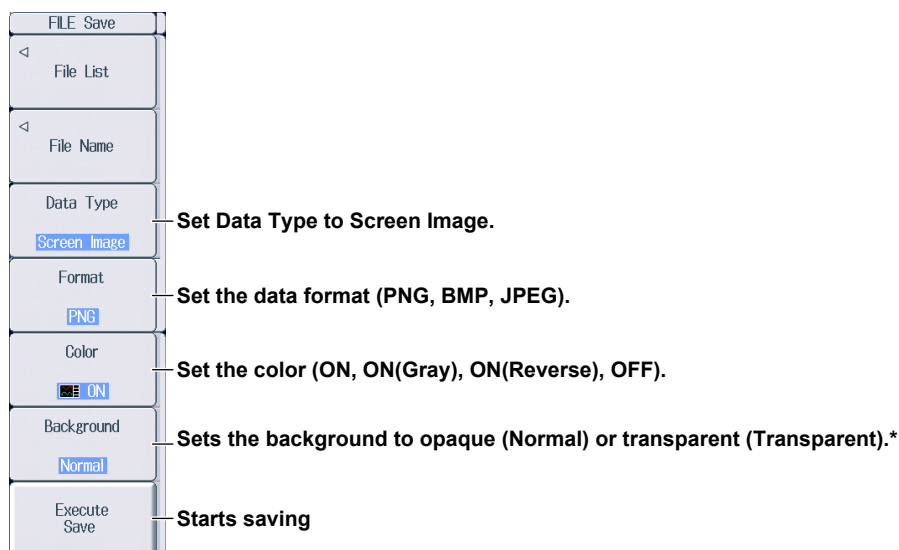

* This appears when the data format is set to PNG.
When the data format is set to JPEG, the frame on/off setting appears.

Setting the Data Format (Format)

Screen captures can be saved in the following data formats. The table below shows the extensions that are automatically assigned to each format and the approximate sizes of files in each format.

Data Format	Extension	File Size ¹
PNG	*.PNG	Approx. 100 KB (approx. 50 KB) ²
BMP	*.BMP	Approx. 2 MB (approx. 150 KB) ²
JPEG	*.JPG	Approx. 250 KB


¹ When Color is set to ON

² The file sizes in parentheses indicate the file size when Color is set to OFF.


Setting the Color (Color)

ON	An screen capture is produced with a 65536-color palette.
ON(Gray)	An screen capture is produced with a 16-color grayscale palette.
ON(Reverse)	The screen background is not produced in color.
OFF	A black-and-white screen capture is produced.


When Data Type Is Snap

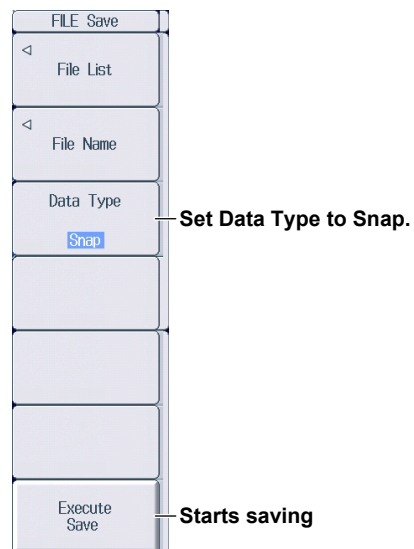

When Data Type Is Measure

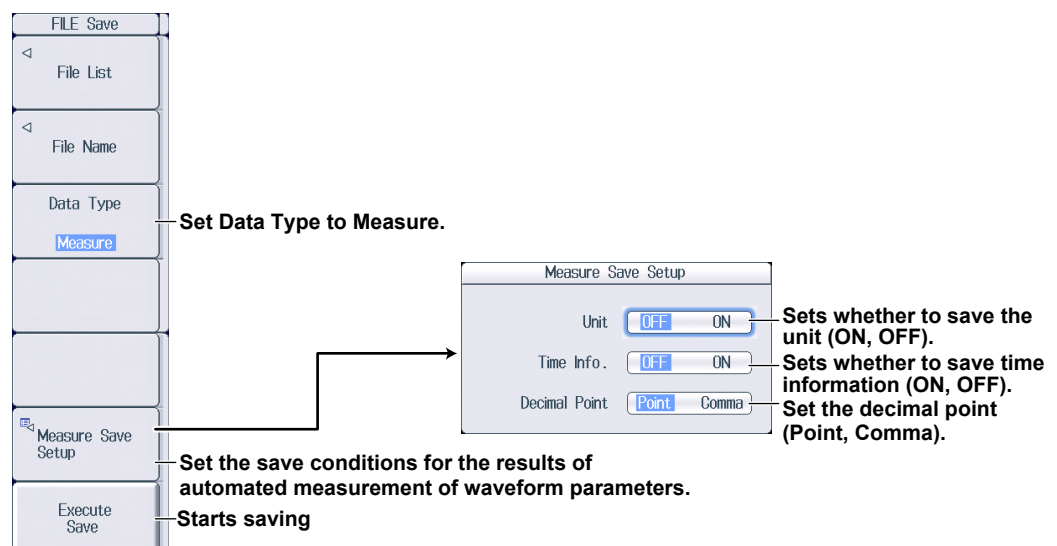

When Data Type Is FFT

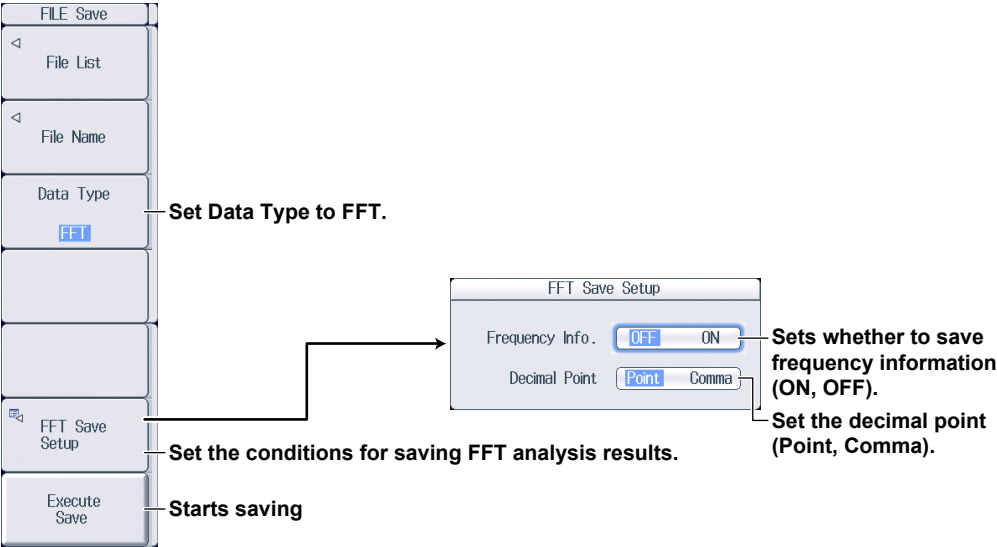

Starting to Save (Execute Save)

Press the **Execute Save** soft key to save the appropriate data file to the specified folder.

22.7 Loading Waveform Data


This section explains the following settings for loading waveform data.

- File to load
- Displaying file information
- Starting to load
- Clearing loaded waveforms

► [Features Guide: “Loading Waveform Data \(Waveform\)”](#)

FILE Waveform Load Menu

Press **FILE** and then the **Waveform** soft key next to Load to display the following screen and menu.

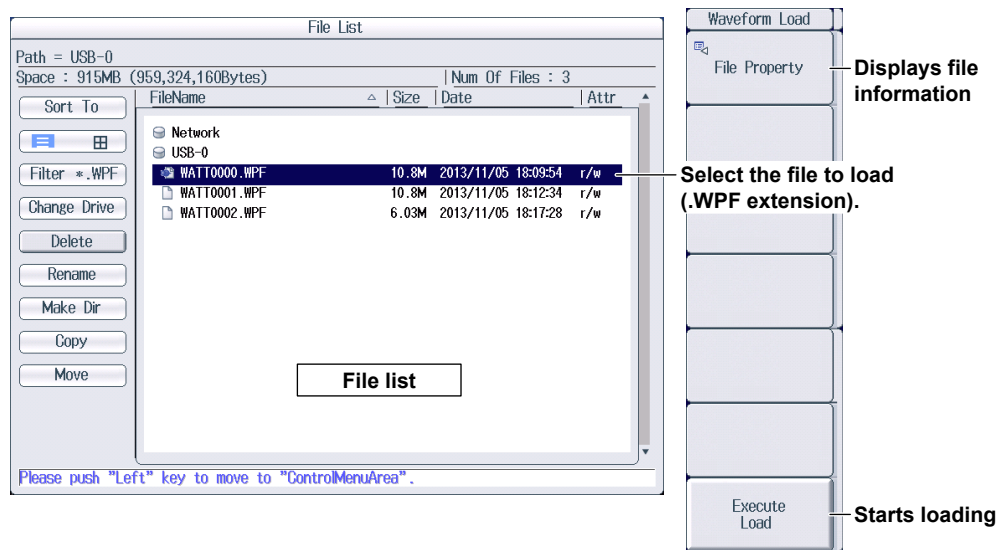

Selecting the File to Load

Select the waveform data file (.WPF extension) to load from the file list. ► [section 22.10](#)

Starting to Load (Execute Load)

Press the **Execute Load** soft key to load the waveform data file from the specified file.

- The setup data in the waveform data file is also loaded. When you start measurement, the loaded waveform data will be cleared, but the setup data that was loaded with the waveform data will remain.
- If the current PX8000 module configuration is different from the modules configuration in the waveform data, you cannot load the waveform data.
- Waveform data saved with a PX8000 model with large memory capacity cannot be loaded in to a model with small memory capacity.

Clearing Loaded Waveforms

Loaded waveforms are cleared in the following situations.

- When waveform acquisition is started with the START/STOP key
- When the Clear History soft key on the HISTORY menu is pressed
- When the PX8000 is initialized

22.8 Loading Setup Data


This section explains the following settings for loading setup data.

- File to load
- Displaying file information
- Starting to load

► [Features Guide: "Loading Setup Data \(Setup\)"](#)

FILE Setup Load Menu

Press **FILE** and then the **Setup** soft key next to Load to display the following screen and menu.

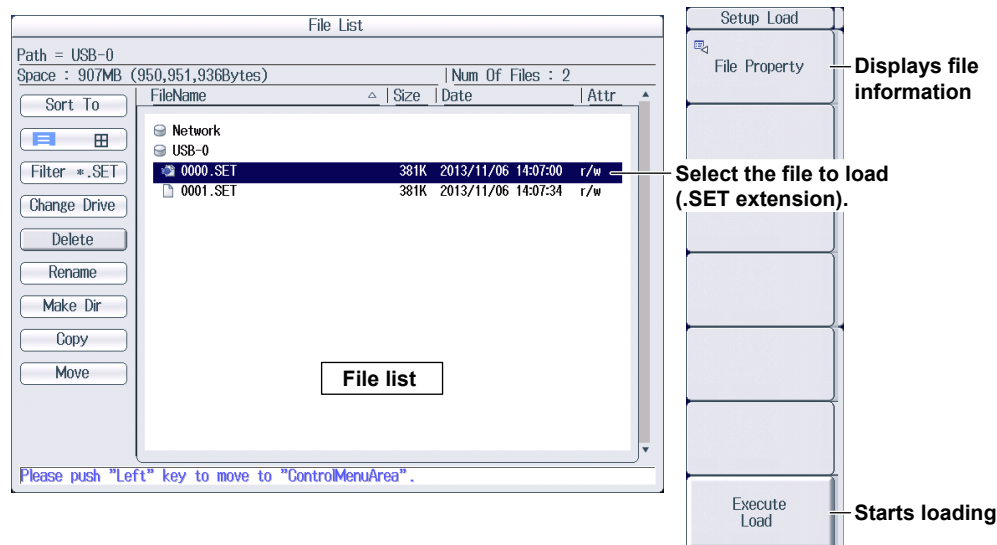

Selecting the File to Load

Select the setup data file (.SET extension) to load from the file list. ► [section 22.10](#)

Starting to Load (Execute Load)

Press the **Execute Load** soft key to load the setup data file from the specified file.

If the current PX8000 module configuration is different from the modules configuration in the setup data, you cannot load the setup data.

22.9 Loading Other Types of Data


This section explains the following settings for loading snapshot waveforms.

- File to load
- Displaying file information
- Starting to load
- Clearing Loaded Waveforms

► [Features Guide: “Loading Other Types of Data \(Others\)”](#)

FILE Others Load Menu

Press **FILE** and then the **Others** soft key next to Load to display the following screen and menu.

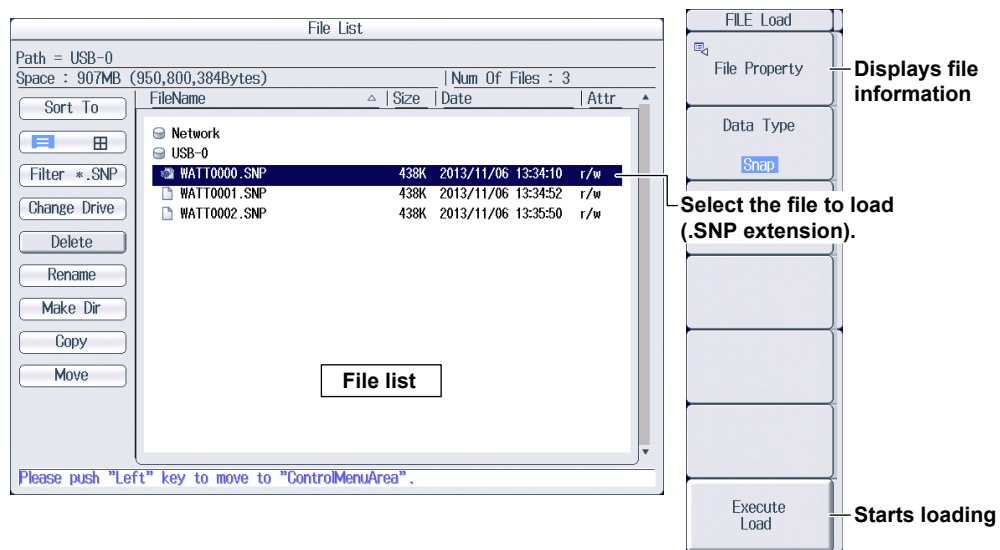

Selecting the File to Load

Select the snapshot data file (.SNP extension) to load from the file list. ► [section 22.10](#)

Starting to Load (Execute Load)

Press the **Execute Load** soft key to load the snapshot waveform data file from the specified file.

Clearing Loaded Waveforms

Loaded waveforms are cleared when you press CLEAR TRACE or when you initialize the PX8000.

22.10 Performing File Operations

This section explains the following settings for performing various file operations from the file list or the file utility menu.

File list

- Sorting
- Display format
- Type of file to list
- Changing the storage medium (drive)
- Deleting files and folders
- Renaming files and folders
- Creating folders (directories)

- Copying files
- Moving files

FILE Utility Menu

- Displaying file information
- Turning file protection on and off
- Selecting files (All Set/All Reset and Set/Reset)

► [Features Guide: "File Operations \(Utility\)"](#)

File List and FILE Utility Menu

1. Press **FILE** and then the **Waveform**, **Numeric**, **Setup**, or **Others** soft key next to Save.
2. Press the **File List** soft key to display the file list and FILE Utility menu.

For details on the FILE Utility menu, see page 22-28.

File List (File List)

File path
Free space

Operation menu cursor
Use the arrow keys (▲▼) to move.

Sort the file list.
Set the display format.
Set the type of files to list.

Change the storage medium (drive).

Delete files and folders.

Rename files and folders.

Create folders (directories).

Copy files and folders.

Move files and folders.

Selection marks

If you want to perform an operation on a group of files at the same time, move the cursor to a file that you want to select, and then press the **SET/RESET** soft key or **SET** to display this icon next to the file.

To select multiple folders, press the **SET/RESET** soft key to display this mark next to the folders. If the cursor is on a folder, pressing **SET** will open the folder. All the files and folders that you have selected up to that point will be canceled.

If you want to perform an operation on a single file, move the cursor to the file you want to select to display this icon next to the file.

FileName	Size	Date	Attr
0000.PNG	62.2K	2013/11/06 13:37:54	r/w
0000.SET	381K	2013/11/06 14:07:00	r/w
0000.WPF	6.03M	2013/11/06 14:08:34	r/w
0000N.CSV	2.74K	2013/11/06 14:08:34	r/w
0001.PNG	147K	2013/11/06 14:08:58	r/w

Total number of files and folders that are contained within the storage medium or folder indicated by the path

File list cursor
Use the arrow keys (▲▼) to move.

FileName	Size	Date	Attr
0001.PNG	147K	2013/11/06 14:08:58	r/w
0001.SET	381K	2013/11/06 14:07:34	r/w
0002.PNG	10.8M	2013/11/05 18:09:54	r/w
WATT0000.CSV	438K	2013/11/06 13:34:52	r/w
WATT0001.WPF	10.8M	2013/11/05 18:12:34	r/w
WATT0001.SNP	438K	2013/11/06 13:35:50	r/w
WATT0002.SNP	6.03M	2013/11/05 18:17:28	r/w
WATT0002.WPF			

Please push "Left" key to move to "ControlMenuArea".

Operation menu ↔ **File list**
Use the arrow keys (◀▶) to switch between the operation areas.

Selects and unselects files and folders

Utility

File Property

Protect ON

Protect OFF

ALL SET


ALL RESET

SET/RESET

Sorting the File List (Sort To)

Select **Sort To** on the operation menu to display the following screen.

- Sort by file name in ascending order. — By Name[▲]
- Sort by file name in descending order. — By Name[▼]
- Sort by file size in ascending order. — By Size[▲]
- Sort by file size in descending order. — By Size[▼]
- Sort by date in ascending order. — By Date[▲]
- Sort by date in descending order. — By Date[▼]

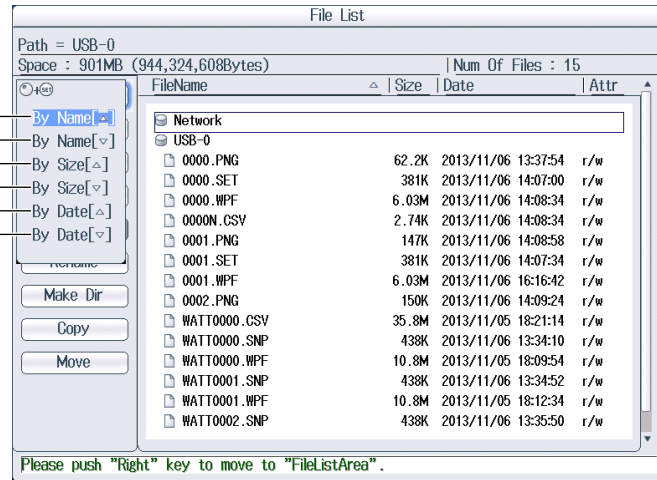


Display Format

Select **display format** on the operation menu to display the following screens.


Press **SET** to switch between display formats.

List Display (≡)

Display format

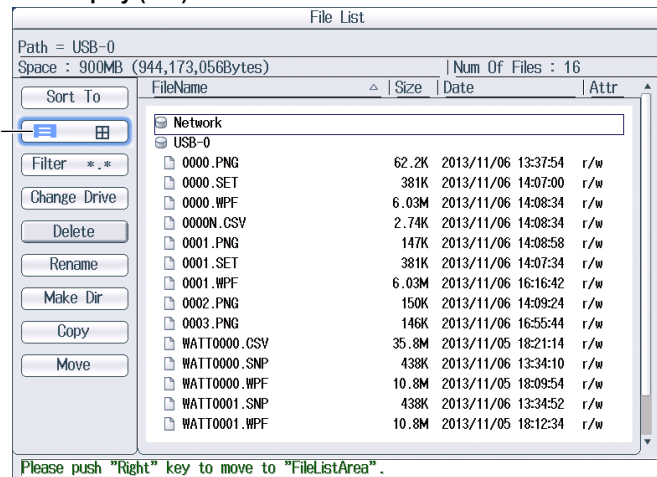

Thumbnail Display (田)

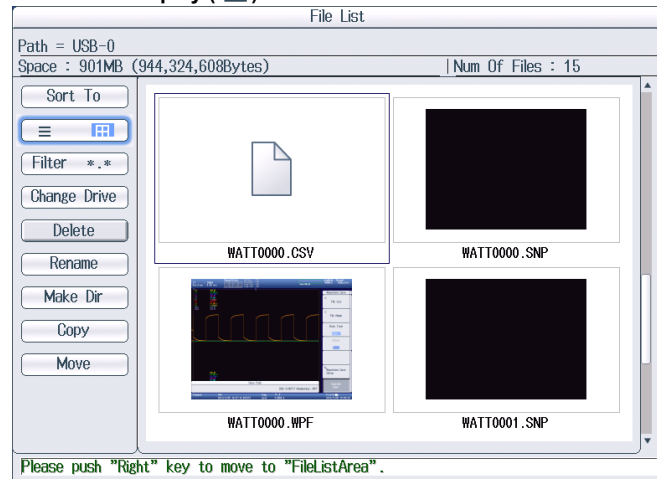


Selecting the Type of File to List (Filter)

Select **Filter** on the operation menu to display the following screen.

Select the type of files to list.

- *.*: All files
- *.WPF: Binary waveform files
- *.CSV: ASCII waveform files
- *.FLD: Floating-point waveform files
- *.SET: Setup files
- *.BMP: Bitmap image files
- *.PNG: PNG image files
- *.JPG: JPEG image files
- *.SNP: Snapshot waveform files
- *.TXT: Text files, custom display configuration files for numeric data, MATLAB waveform files

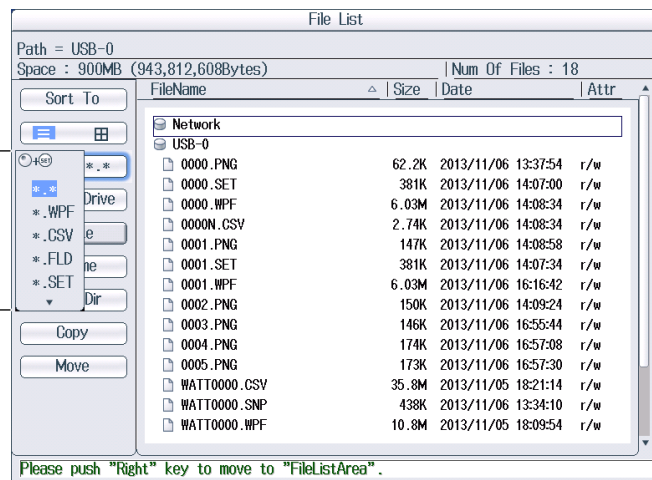


Changing the Storage Medium or Drive (Change Drive)

Select **Change Drive** on the operation menu to display the following screen.

Select the storage medium (drive).

- SD-1: SD card
- USB-0: The first detected USB storage medium
- USB-1: The second detected USB storage medium
- Network: Network Drive

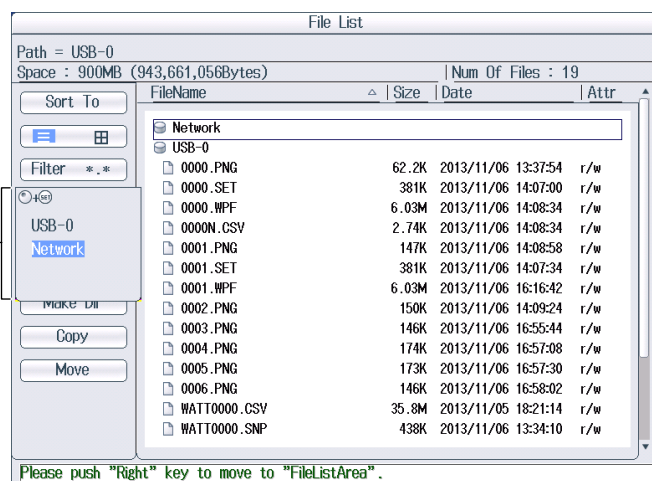


Note

You can also change the storage medium by highlighting the storage medium (drive) you want to change to in the file list and pressing **SET**.

Deleting Files and Folders (Delete)

1. Select the file or folder that you want to delete from the file list.
2. Select **Delete** on the operation menu to display the following screen.

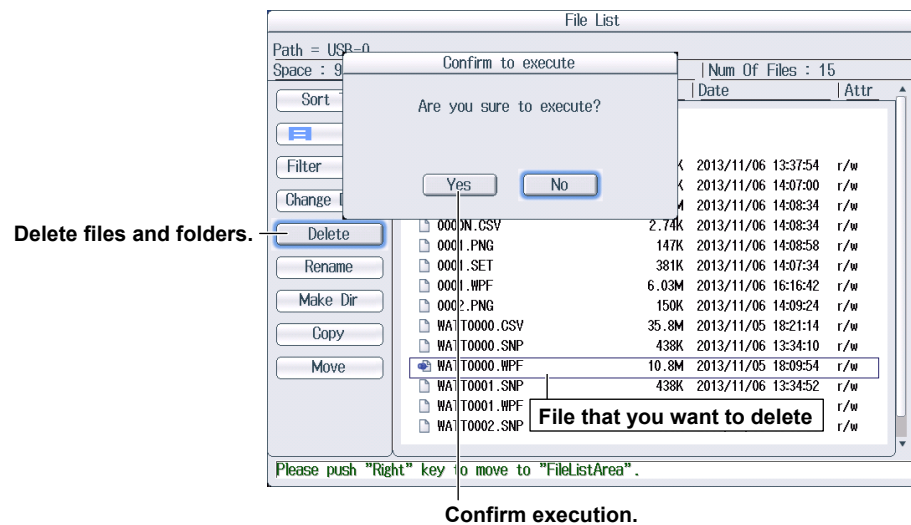


Note

- To delete multiple files or folders that are in the file list at the same time, move the cursor to the file or folder that you want to delete, and then carry out the following operations.
Files: Press **SET** or the **SET/RESET** soft key on the Utility menu.
Folders: Press the **SET/RESET** soft key on the FILE Utility menu. If the cursor is on a folder, pressing **SET** will open the folder. All the files and folders that you have selected up to that point will be canceled.
- You can abort file deleting. However, files that are already being processed are not applicable.

Renaming Files and Folders (Rename)

1. Select the file or folder that you want to rename from the file list.
2. Select **Rename** on the operation menu to display the following screen.

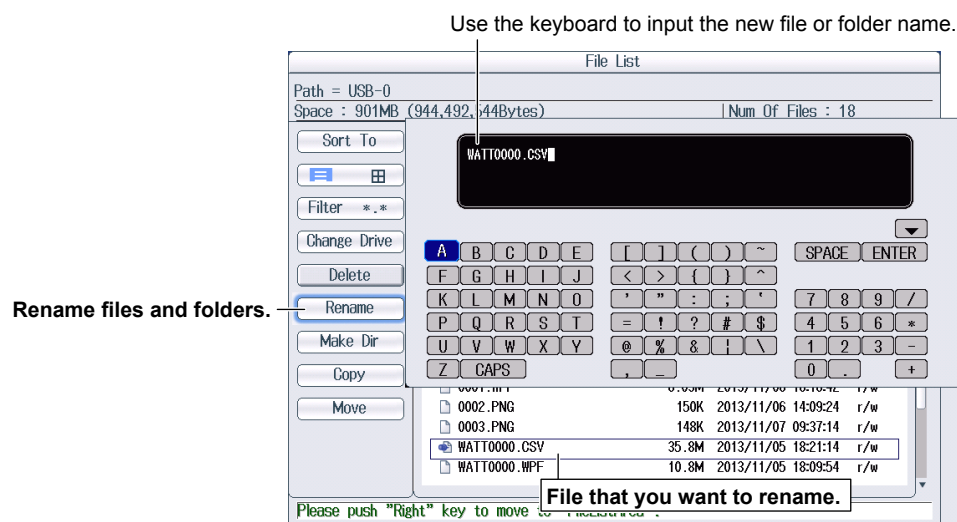


Press **ENTER** on the keyboard or the **Enter** soft key to confirm the name you entered.

Making Folders (Make Dir)

1. Select the drive or folder in the file list that you want to make the new folder in.
2. Select **Make Dir** on the operation menu to display the following screen.


Create folders (directories).

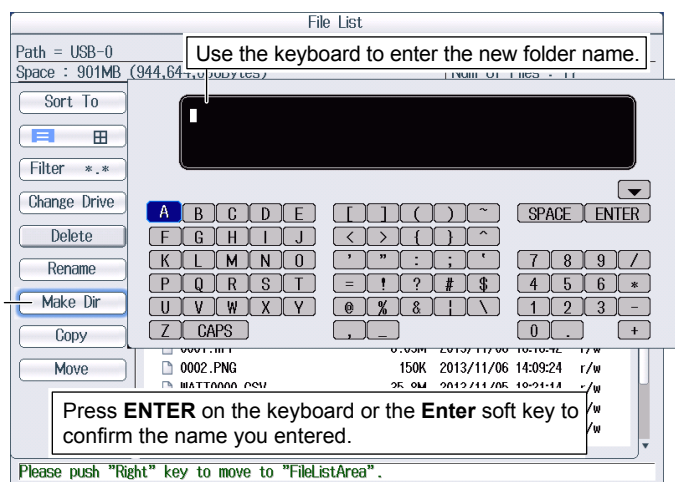

Copying Files (Copy)


1. Select the file that you want to copy from the file list.
2. Select **Copy** on the operation menu to display the following screen.

Copies the selected files and folders

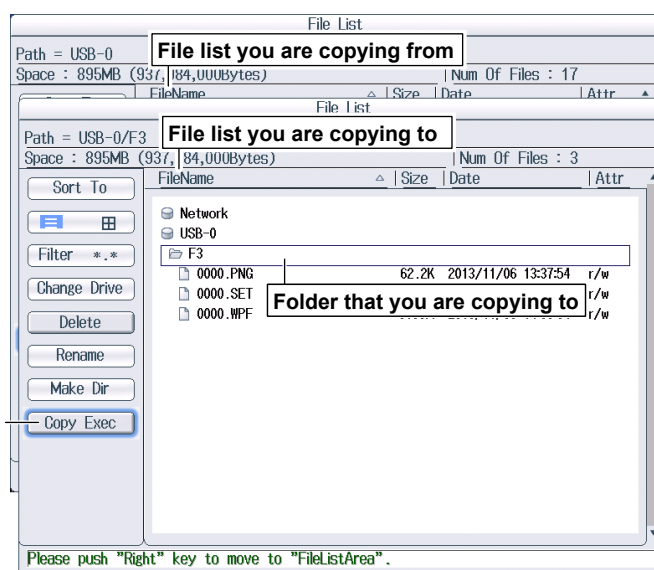

3. Select the drive or folder on the file list that you are copying to.
4. Select **Copy Exec** on the operation menu to display the following screen.

Confirm execution.

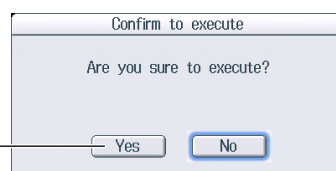


Note


- The procedure for selecting multiple files or folders at the same time to copy them is the same as the procedure for selecting multiple files or folders at the same time to delete them. For more details, see the note on page 22-25.
- You can abort file copying.

Moving Files (Move)

1. Select the file that you want to move from the file list.
2. Select **Move** on the operation menu to display the following screen.

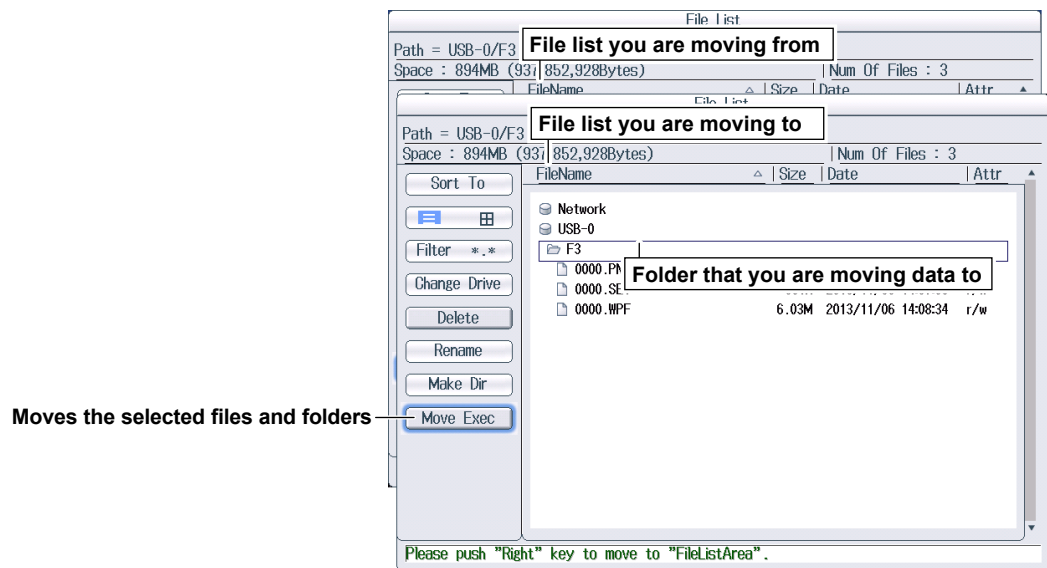



3. Select the drive or folder in the file list that you are moving to.
4. Select **Move Exec** on the operation menu to display the following screen.

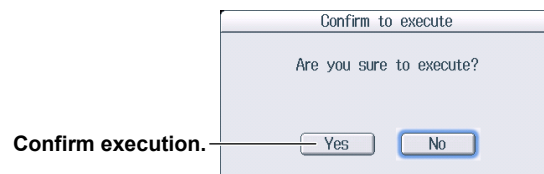

Note

The procedure for selecting multiple files or folders at the same time to move them is the same as the procedure for selecting multiple files or folders at the same time to delete them. For more details, see the note on page 22-25.

FILE Utility Menu

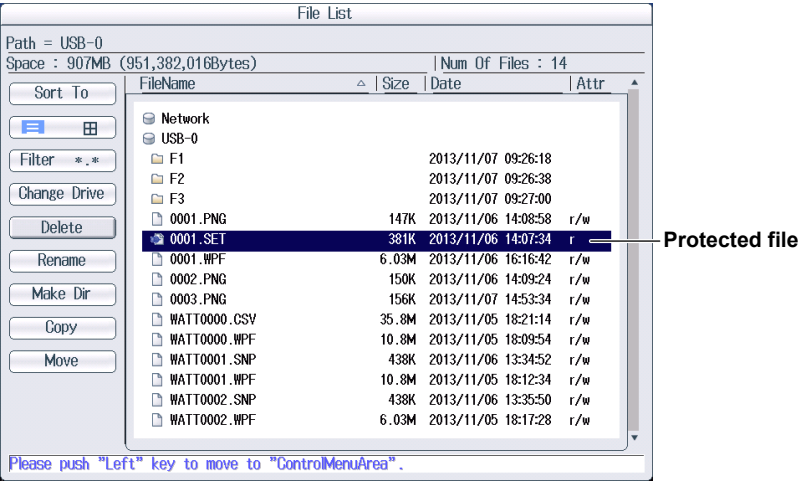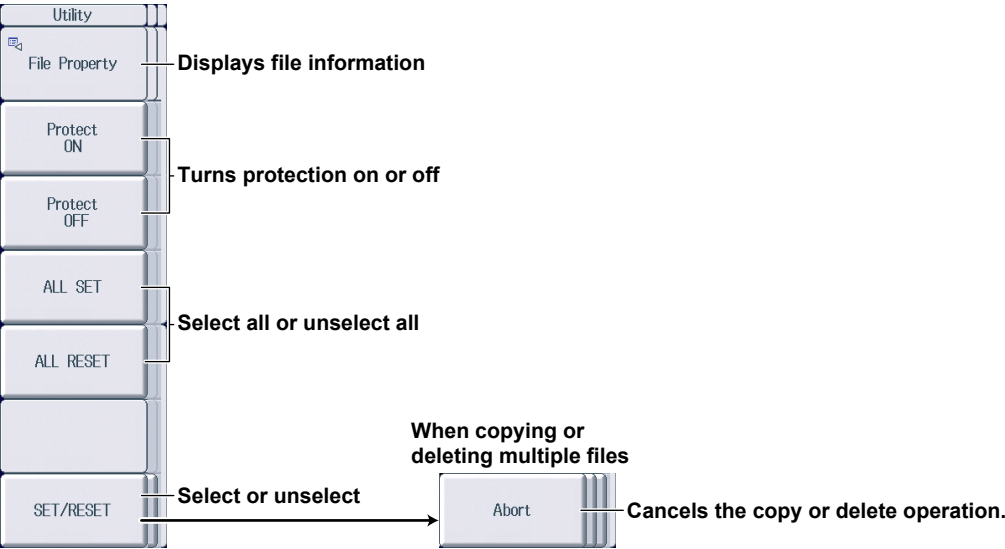

Turning Protection On or Off (Protect ON/OFF)

These soft keys turn protection on and off for the selected file. The change is reflected in the file attributes, displayed under the Attr column in the file list.

Protection	File Attribute	Description
ON	r	File protection is on for the selected file. The file can be read from. Writing is not allowed. Deleting is also not allowed.
OFF	r/w	File protection is off for the selected file. The file has read and write access.

ALL SET and ALL RESET

- ALL SET: When a medium, folder, or file is highlighted in the file list, pressing this soft key selects all the files and folders in the corresponding medium or folder. Selection marks (see page 16-19) are displayed to the left of the selected files and folders.
- ALL RESET: Pressing this soft key clears all the selected files and folders.

SET/RESET

This soft key selects the file or folder in the file list that is highlighted or clears the selection. Selection marks (see page 22-22) are displayed to the left of the selected files.


23.1 Connecting the PX8000 to a Network

This section explains how to connect the PX8000 to a network.

Ethernet Interface Specifications

There is a 1000BASE-T port located on the side panel of the PX8000.

Item	Specifications
Ports	1
Electrical and mechanical specifications	IEEE802.3 compliant
Transmission system	Ethernet (1000BASE-T, 100BASE-TX, 10BASE-T)
Communication protocol	TCP/IP
Supported services	Server: FTP and VXI-11 Client: FTP (Net Drive), SNMP, DHCP, and DNS
Connector type	RJ-45

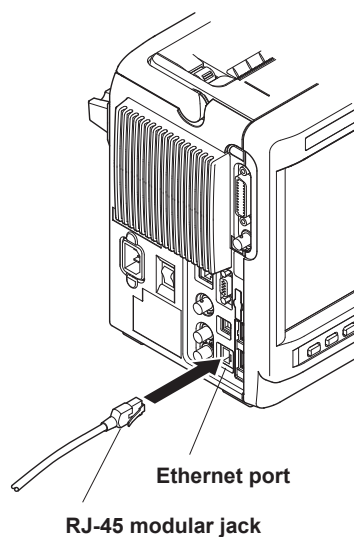

Items Required to Connect the PX8000 to a Network

Cable


Use one of the following types of network cable that conforms to the transfer speed of your network.

- A UTP (Unshielded Twisted-Pair) cable
- An STP (Shielded Twisted-Pair) cable

Connection Procedure


To Connect to a PC over a Network

1. Turn off the PX8000.
2. Connect one end of a UTP (or STP) cable to the ETHERNET 1000BASE-T port on the side panel.
3. Connect the other end of the UTP (or STP) cable to a hub or router.
4. Turn on the PX8000.

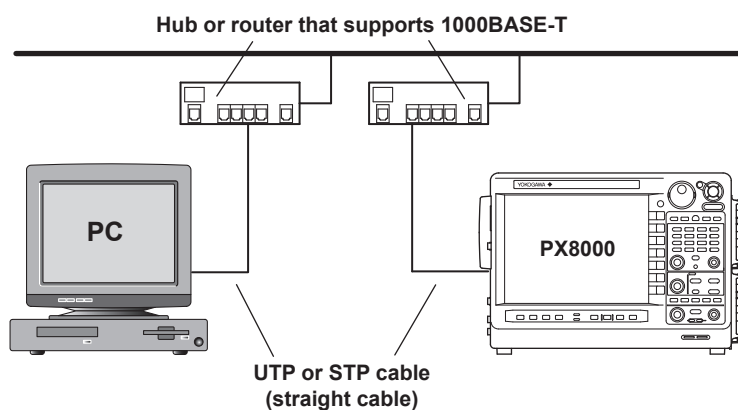

To Connect to a PC through a Hub or Router

1. Turn off the PX8000.
2. Connect one end of a UTP (or STP) cable to the ETHERNET 1000BASE-T port on the side panel.
3. Connect the other end of the UTP (or STP) cable to a hub or router.
4. Connect the PC to the hub or router in the same way.
5. Turn on the PX8000.

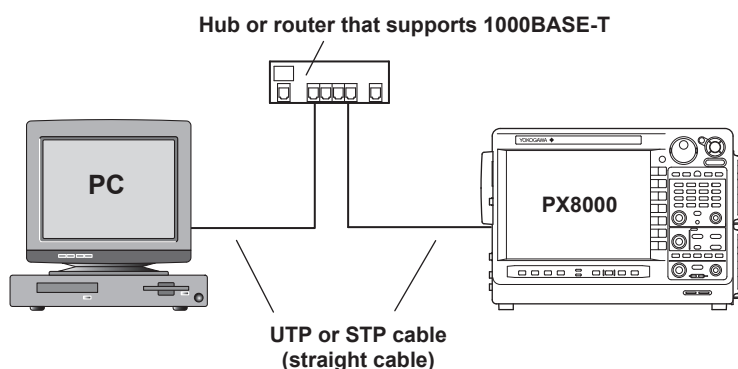

Note

- Use a hub or router that conforms to the transfer speed of your network.
 - When you connect a PC to the PX8000 through a hub or router, the PC must be equipped with an auto switching 1000BASE-T/100BASE-TX/10BASE-T network card.
 - Do not connect the PX8000 to a PC directly. Direct communication without a hub or router is not guaranteed to work.
-

23.2 Configuring TCP/IP Settings


This section explains the following TCP/IP settings for connecting to a network.

- DHCP (IP address, subnet mask, and default gateway)
- DNS (domain name, DNS server IP address, and domain suffix)

► [Features Guide: "TCP/IP \(TCP/IP\)"](#)


UTILITY Network Menu

Press **UTILITY** and then the **Network** soft key to display the following menu.

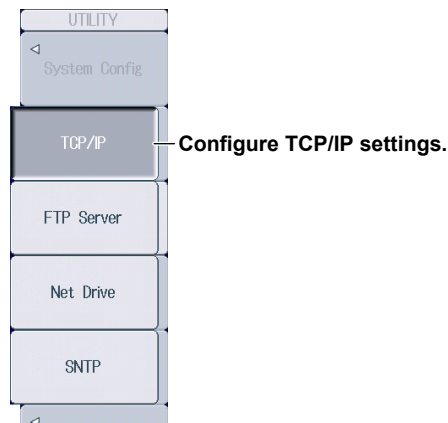

Configuring TCP/IP Settings (TCP/IP)

Press the **TCP/IP** soft key to display the following screen.

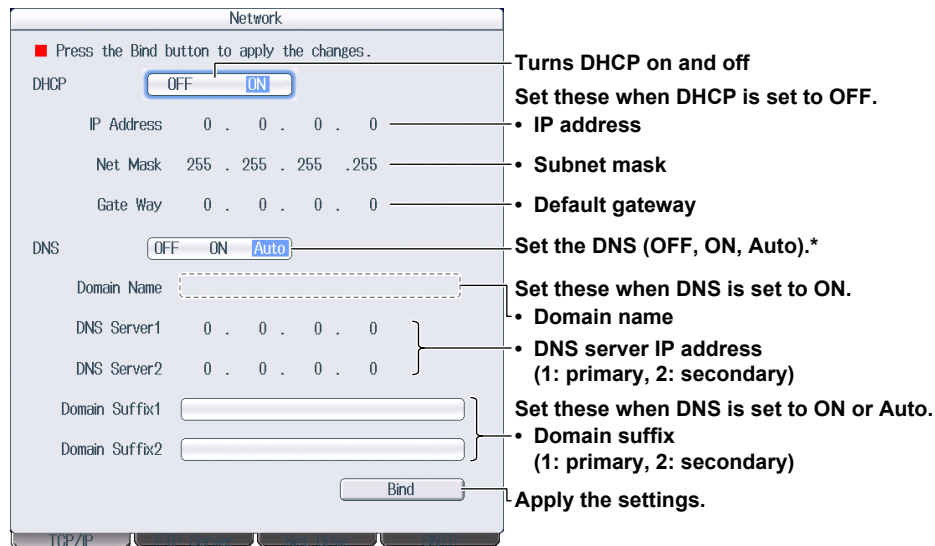

* Auto is displayed when DHCP is on.

DNS Settings (DNS)

OFF: DNS is disabled.

ON: DNS is enabled. Set the domain name, and the DNS server's primary and secondary IP addresses and domain suffixes.

Auto: DNS is enabled. Set the domain suffix. The domain name and the DNS server IP addresses are set automatically. This option can only be selected when DHCP is on.

23.3 Accessing the PX8000 from a PC (FTP Server)


This section explains the following settings for accessing the PX8000 from a PC on a network.

- User name
- Password
- Timeout
- Starting an FTP Client

► [Features Guide: “FTP Server \(FTP Server\)”](#)


UTILITY Network Menu

Press **UTILITY** and then the **Network** soft key to display the following menu.

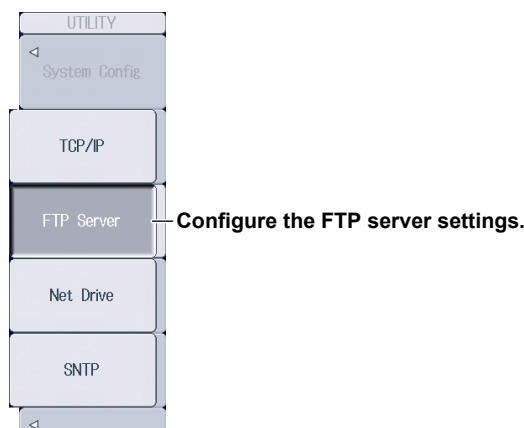

Configuring FTP Server Settings (FTP Server)

Press the **FTP Server** soft key to display the following screen.

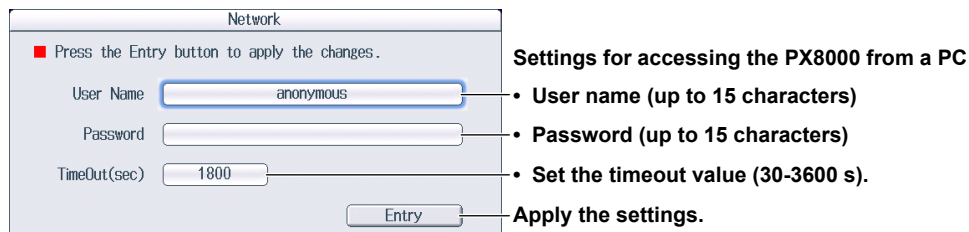

Starting an FTP Client

Start an FTP client on a PC.

Enter the user name and password that you entered on the screen shown above to connect to the PX8000.

Note

If you set the user name to “anonymous,” you can connect to the PX8000 without entering a password.

23.4 Connecting to a Network Drive


This section explains the following settings for accessing a network drive through an Ethernet connection to load or save various PX8000 data.

- FTP server (file server)
- Login name
- Password
- Turning FTP passive mode on and off
- Timeout
- Connecting to and disconnecting from network drives

► [Features Guide: “Network Drive \(Net Drive\)”](#)


UTILITY Network Menu

Press **UTILITY** and then the **Network** soft key to display the following menu.

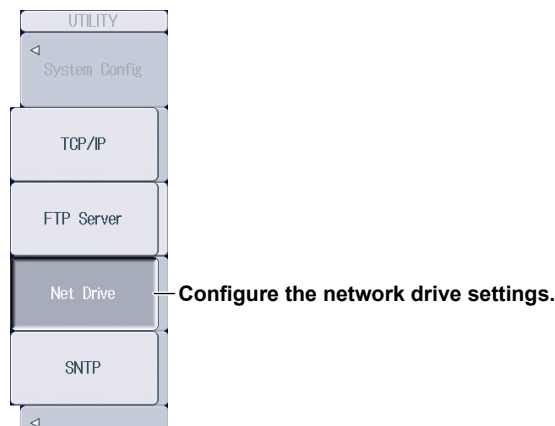

Configuring a Network Drive and Connecting to It (Net Drive)

Press the **Net Drive** soft key to display the following screen.

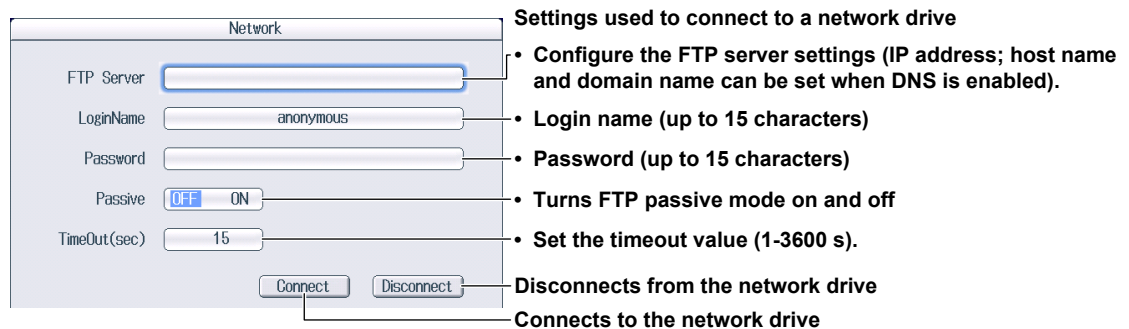

23.5 Using SNTP to Set the Date and Time


This section explains how to use SNTP to set the PX8000's date and time.

- SNTP server
- Timeout
- Executing time adjustment
- Automatic adjustment

► [Features Guide: "SNTP \(SNTP\)"](#)


UTILITY Network Menu

Press **UTILITY** and then the **Network** soft key to display the following menu.

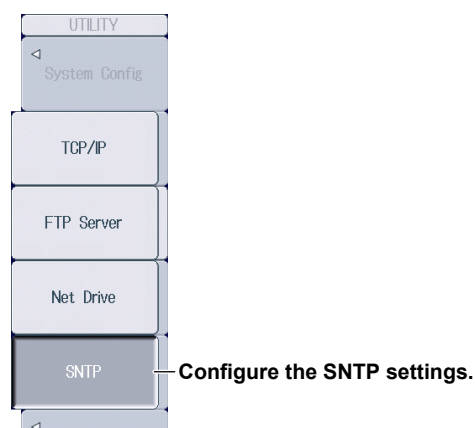

Configuring SNTP Settings (SNTP)

Press the **SNTP** soft key to display the following screen.

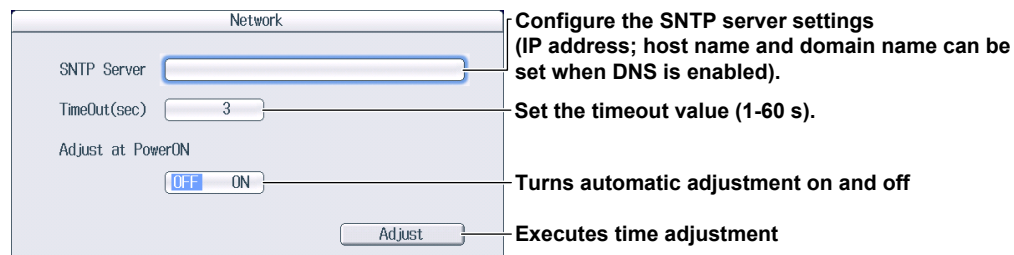

24.1 Calibrating the PX8000

This section explains how to calibrate the PX8000. Execute calibration when you want to make accurate measurements.

► [Features Guide: “Calibration \(Zero-level compensation, CAL\)”](#)

CAL Menu

Press **SHIFT+DISPLAY MODE** (CAL) to display the following menu.

CAL	
Execute Calibration	Executes calibration
Cal at End for Elements OFF ON	Turns on and off the calibration that is performed when a measurement is completed on an element
Cal on Start for Auxiliaries OFF AUTO	Set the calibration that is performed after starting signal acquisition on AUX modules (OFF, AUTO). This command does not appear if AUX modules are not installed.

24.2 Using the NULL Feature

This section explains the following settings for the NULL feature.

- Turning NULL value subtraction on and off
Turning on and off at once, setting each channel separately
- Turning NULL value updating on and off
Turning on and off at once, setting each channel separately
- Enabling and Disabling the NULL Feature

► [Features Guide: “NULL Feature \(NULL SET\)”](#)


Configuring NULL Feature Settings

Press **SHIFT+NULL** (NULL SET) to display the following screen.

To collectively set all the channels of installed modules, set the items in the All row.

Collectively turns NULL value subtraction on and off

Collectively turns NULL value updating on and off

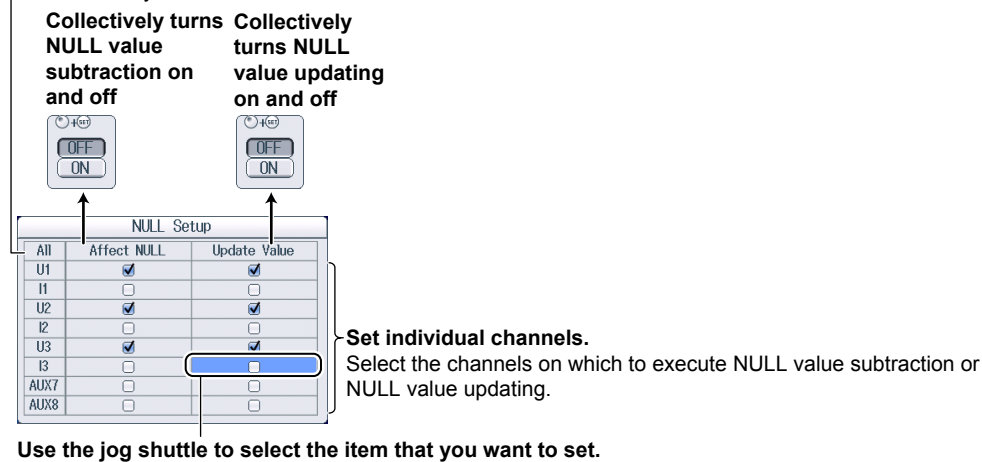

Set individual channels.
Select the channels on which to execute NULL value subtraction or NULL value updating.


Use the jog shuttle to select the item that you want to set.

Enabling and Disabling the NULL Feature

Press **NULL**. The NULL feature is executed, and a NULL indicator appears in the element information display area on the right side of the screen.

- The NULL value of each signal is used for those channel signals whose NULL feature is set to ON.
- If you press the NULL key again, the NULL feature is disabled, and the NULL indicator disappears.

NULL indicators

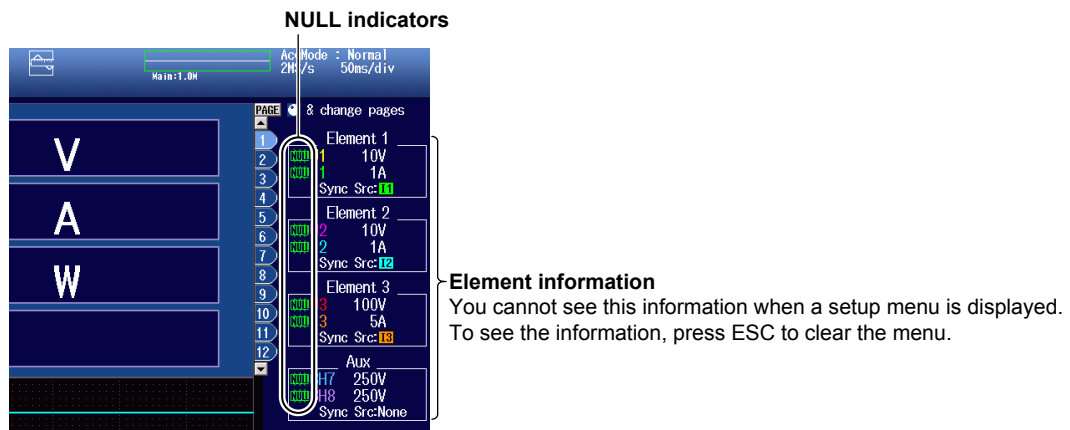

Element information
You cannot see this information when a setup menu is displayed.
To see the information, press ESC to clear the menu.

Note

If the measured value of the input signal used as a NULL value is not available (no measured value or measurement error), even if “NULL value updating” of the signal is set to ON, an error will occur because the NULL value will not be updated.

24.3 Setting Time Synchronization (Option)


This section explains the following settings for synchronizing the PX8000 to GPS time.

- IRIG format
- Modulation type
- Input impedance

► [Features Guide: “Time Synchronization Feature \(Time Synchro; optional\)”](#)

UTILITY System Config Time Synchro Menu

Press **UTILITY**, the **System Config** soft key, and then the **Time Synchro** soft key to display the following menu.

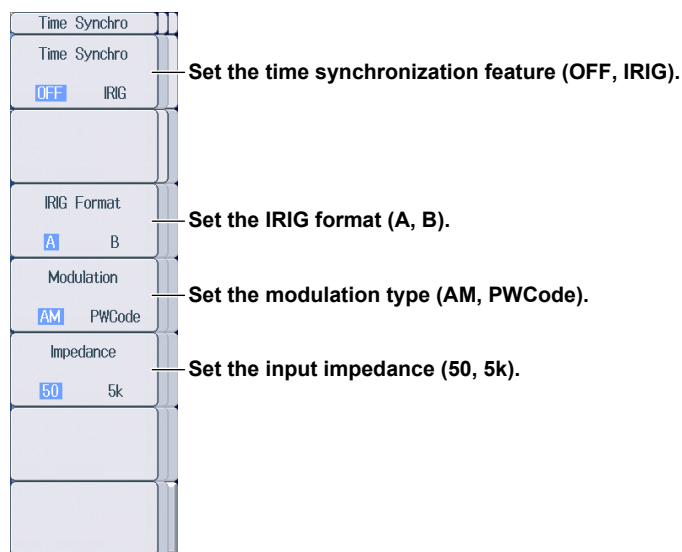

Note

To enable the changes that you have made to the time synchronization settings, restart the PX8000.


24.4 Changing the Message, Menu, and USB Keyboard Languages

This section explains the settings that you can use to change the message, menu, and USB keyboard languages.

► [Features Guide: “Language \(Language\)”](#)
[“USB Keyboard Language \(USB Keyboard\)”](#)


UTILITY System Config Menu

Press **UTILITY**, and then the **System Config** soft key to display the following menu.

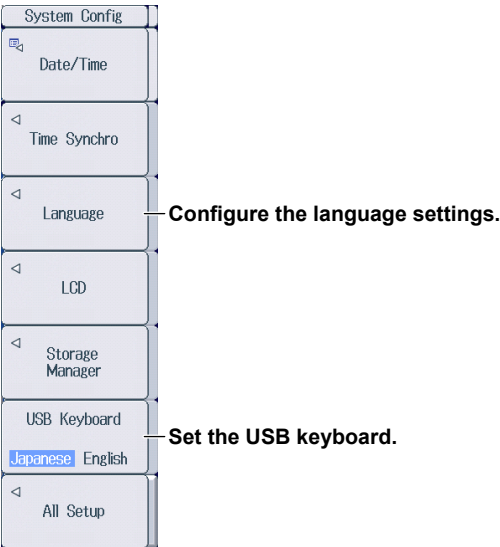

Setting the Language (Language)

Press the **Language** soft key to display the following menu.

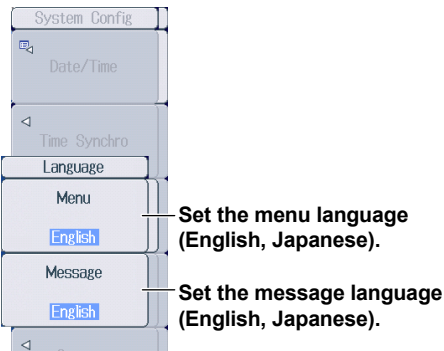

Note _____
Some terminology is always displayed in English.

Setting the USB Keyboard Language (USB Keyboard)

You can use the following keyboards that conform to USB Human Interface Devices (HID) Class Ver. 1.1.
English: 104-key keyboards
Japanese: 109-key keyboards

For details on how PX8000 keys are mapped to the keys on a USB keyboard, see appendix 10 in the Features Guide, IM PX8000-01EN.

24.5 Adjusting the Backlight

This section explains the following settings for adjusting the backlight.

Turning off the backlight


Automatically turning off the backlight

Adjusting the brightness

► [Features Guide: “Adjusting the LCD \(LCD\)”](#)

UTILITY System Config LCD Menu

Press **UTILITY**, the **System Config** soft key, and then the **LCD** soft key to display the following menu.

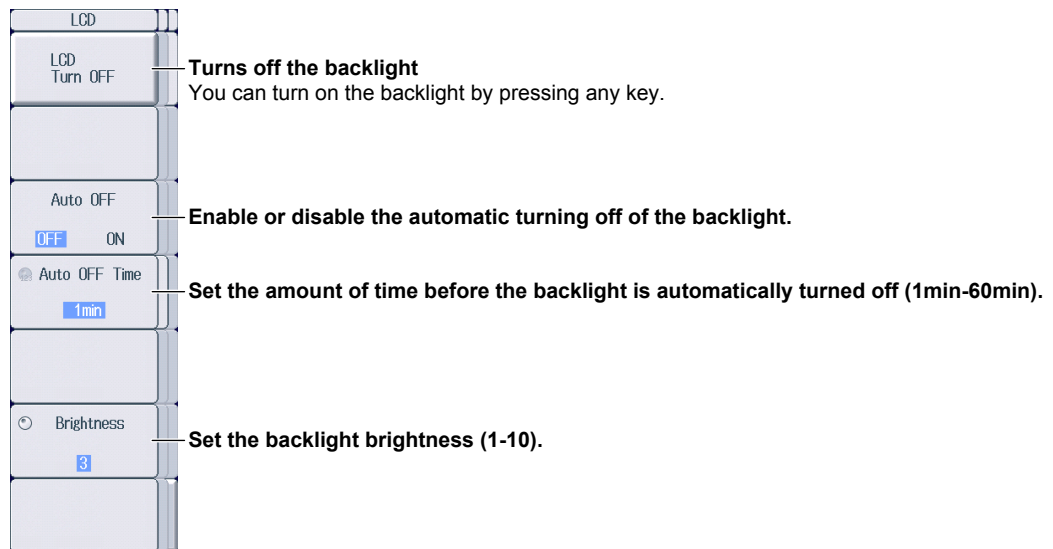


24.6 Initializing the Settings

This section explains how to initialize the PX8000 settings to their factory default values.

► [Features Guide: “Initializing Settings \(Initialize\)”](#)

UTILITY System Config All Setup Menu

Press **UTILITY**, the **System Config** soft key, and then the **All Setup** soft key to display the following menu.

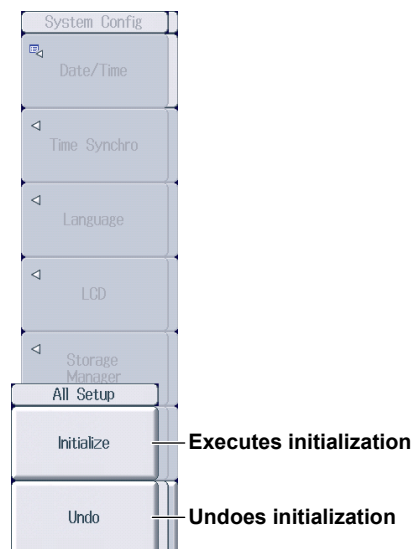

24.7 Configuring the Environment Settings


This section explains the following environment settings.

- Action to perform at power on
- Terminal (external I/O terminal) signal
- Display settings
Font size, menu background color, scale value display, numeric display frame, number of digits to display for numeric data, intensity
- Key and knob control settings
Turning the click sound on and off, start and stop response time, key lock type and release type
- Frequency display when the measured frequency is less than the lower limit
- AUX display when the measured pulse frequency is less than the lower limit
- Analysis settings
Cursor read mode

► [Features Guide: “Environment Settings \(Preference\)”](#)


UTILITY Preference menu

Press **UTILITY** and then the **Preference** soft key to display the following menu.

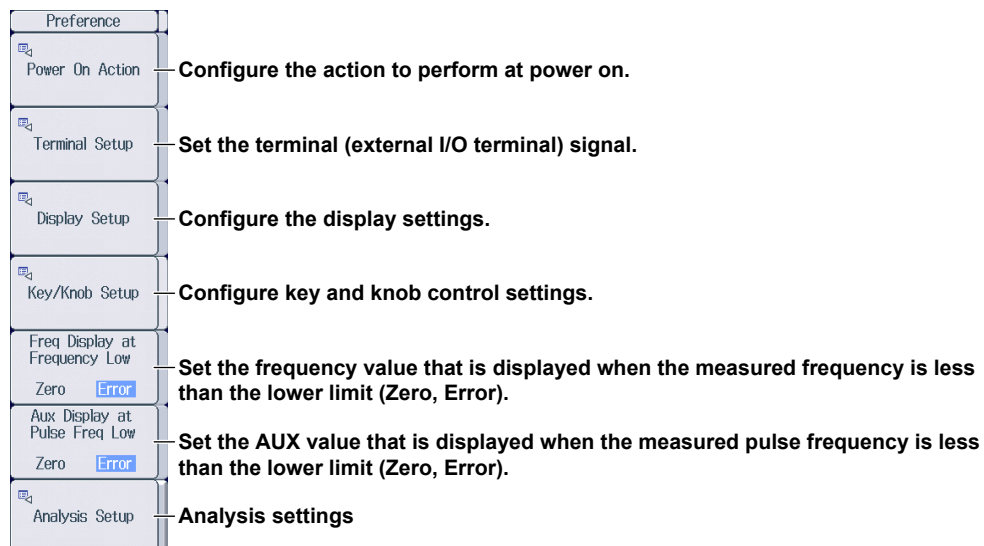


Setting the Action to Perform at Power On (Power On Action)

Press the **Power On Action** soft key to display the following screen.

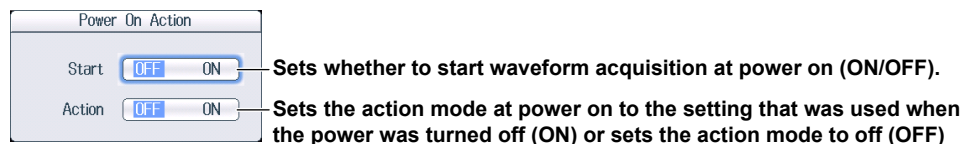

Setting the Terminal (External I/O Terminal) Signal Settings (Terminal Setup)


Press the **Terminal Setup** soft key to display the following screen.

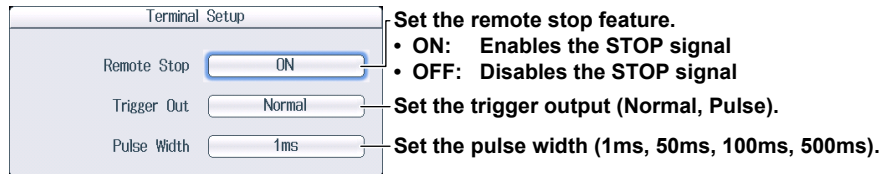

Configuring the Display Settings (Display Setup)

(Font size, menu background color, scale value display, numeric display frame, number of digits to display for numeric data, intensity)


Press the **Display Setup** soft key to display the following screen.

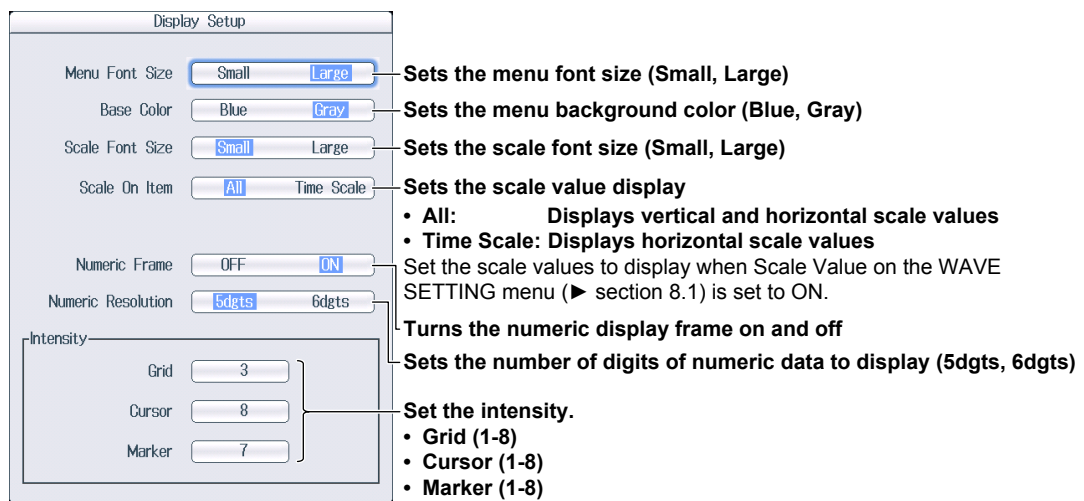

Configuring Key and Knob Control Settings (Key/Knob Setup)


(Turning the click sound on and off, start and stop response time, key lock type and release type)

Press the **Key/Knob Setup** soft key to display the following screen.

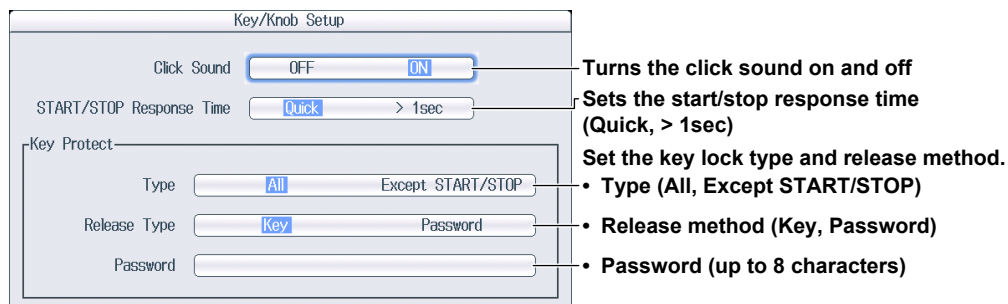

Configuring Analysis Settings (Analysis Setup)

Press the **Analysis Setup** soft key to display the following screen.

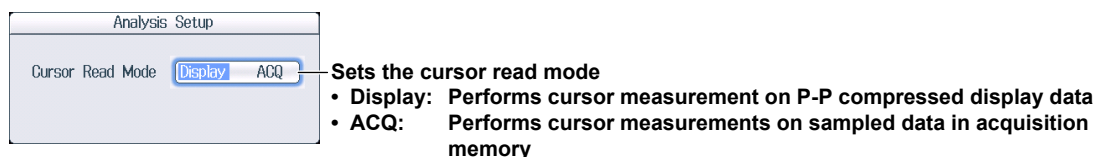

24.8 Storing and Recalling Setup Data

This section explains how to store the PX8000 settings to the internal memory and how to recall settings from the internal memory.

► [Features Guide: “Storing and Recalling Setup Data \(Setup Data Store and Recall\)”](#)

UTILITY Store/Recall Menu

Press **UTILITY** and then the **Setup Data Store/Recall** soft key to display the following menu.

Store/Recall	
No. 2	Specify the store/recall number (1-16).
2013/11/11 11:57:02	Date and time when the data was stored*
Comment	Set comments.
Store Exec	Starts storing
Recall Exec	Starts recalling*
Clear	Clears the stored setup data*

* This appears when data is stored in the internal memory at the specified store/recall number.

24.9 Locking the Keys

This section explains how to lock the panel keys, which prevents you from unintentionally changing the current state of the PX8000.

► [Features Guide: “Key Lock \(KEY PROTECT\)”](#)

Key Lock (KEY PROTECT)

Press **KEY PROTECT** to lock the panel keys. The KEY PROTECT key illuminates. When the keys are locked, pressing any keys other than **KEY PROTECT** has no effect. Press **KEY PROTECT** again to release the key lock and enable the panel keys. The KEY PROTECT key turns off.

Note

When the keys are locked, you cannot use a USB mouse or keyboard to operate the PX8000 either.

25.1 Messages and Corrective Actions

Message

Messages may appear on the screen during operation. This section describes the error messages and how to respond to them. With a few exceptions, you can display the messages in the language that you specify through the operations explained in section 24.4. If servicing is necessary to solve the problem indicated by a message, contact your nearest YOKOGAWA dealer.

In addition to the following error messages, there are also communications error messages. These messages are explained in the Communication Interface User's Manual (IM PX8000-17EN).

Information

Code	Message	Chapter or Section
53	Initializing is in progress.	24.6
54	Initializing has been completed.	24.6
55	Undo is in progress.	24.6
56	Undo has been completed.	24.6
59	Calibration is running...	24.1
60	Calibration is complete.	24.1
61	Media format is running.	22.2
62	Media format is complete.	22.2
64	File access is aborted.	—
65	Executed the firmware overwriting of the frequency module.	25.3
66	Overwriting firmware of the frequency module...	25.3
67	Key response time is more than 1 second. Push it more than 1 second.	24.7
68	Executed the firmware overwriting of the built-in parts.	25.3
69	Overwriting the built-in parts firmware.	25.3
70	Exit from GO/NO-GO mode.	Chapter 17
71	Image printing was aborted.	21.2
72	Completed action.	18.1
73	Aborted the search.	Chapter 19, section 20.2
74	Executed the search, but no record was found that matched the conditions.	Chapter 19, section 20.2
75	Executed the search, but no record was found that matched the pattern.	Chapter 19, section 20.2
77	Aborted the statistical measurement.	14.2, 14.3
80	Input module configuration was changed. Relevant settings have been initialized.	Appendix 11*
84	Turned on pressing the RESET key. Will initialize.	Appendix 11*
85	The instrument is set to remote mode by the communication control. Press the SHIFT + CLEAR TRACE key to change to local mode.	—
86	Push 'Zoom Mag' knob or 'Zoom Position' knob when change a target window.	12.1
87	Sensed the firmware version change. Will initialize.	Appendix 11*
94	Executing abort process. It takes a few seconds.	—
96	Calibration failure of power measurement element has occurred. Power-supply frequency exceeded acceptable range for calibration.	24.1

* Features Guide, IM PX8000-01EN

25.1 Messages and Corrective Actions

Code	Message	Chapter or Section
97	The history has been cleared due to one of the following reasons. - Wiring was changed. - Element Independent was changed. - Ext Sensor for Current Module or sense type for Aux Module was changed. - Executed "Elements Copy to" or "Aux Copy to".	1.1, 2.2, 2.4, 2.7
98	A module, which accuracy is not guaranteed, is installed. Or pairs of modules, which accuracy is not guaranteed, is installed. Check modules on the overview display (UTILITY-Overview).	25.3

File Errors

Code	Message	Chapter or Section
500	File access failure.	—
501	Invalid file name. The name contains prohibited characters, or file name is duplicated.	22.3, chapter 24*
502	Pass name over maximum number of characters. Full pass name should under 255 characters.	—
504	Out of disk space.	22.10
505	File not found. Check the file.	22.10
506	Duplicate file or directory name. Change the name.	22.10
507	The file name is not set. Set the file name.	22.3
508	Save data not found. Check for presence of data and channel.	22.3, 22.6
509	File system failure.	—
510	Cannot load this file format. Files stored on other models cannot be loaded.	22.7
511	File is now being accessed. Execute after access is made.	—
512	Cannot be executed while running. Press the START/STOP key to stop acquisition.	4.2
513	The specified file cannot be loaded on this Firmware version or this model.	22.7
514	No ch is displayed. Turn ON the display of the appropriate channel.	22.3
517	Unknown file format.	Chapter 22
518	Writing prohibited in the media. Unlock write protection of the media.	—
519	Cannot save in this format at the current record length. Specify a range and save a section of the data. * Cannot create a file of size 2 GB or larger.	22.3
520	Media error.	22.1
521	Directory can not be deleted.	22.1
522	Cannot load these files on a network drive. - The File which larger than 50 Mbyte. - The File which is saved by HistoryAll format. Copy the file to the local drive before loading it.	23.3
530	Assigned path does not exist. Check the network setting and configuration.	Chapter 23
531	Assigned file does not exist. Check the network setting and configuration.	Chapter 23
532	Assigned path does not exist. Check the network setting and configuration.	Chapter 23
533	Writing prohibited in this file.	22.10
534	An error occurred while network access. Confirm network conditions.	Chapter 23
535	Current path is not suitable. Set other path while use action on trigger.	22.3

* Features Guide, IM PX8000-01EN

Code	Message	Chapter or Section
536	Destination path is same as source path, or sub folder of source path.	—
538	Module configuration is not matched, so it couldn't loaded. Configuration of saved data can see by File property.	22.7
539	Module configuration is not matched, so it couldn't loaded. Configuration of saved data can see by File property.	22.7
541	Cannot detect the medium. Check the presence of the medium.	22.1
544	Cannot execute file operations or initialization while measure is in progress. To execute, wait for the end of measure or turn measure off.	14.1
545	Data read error.	—
547	Cannot execute file operations or initialization while numeric calculations are in progress. To execute, wait for the end of numeric calculation or turn numeric off.	7.1
548	Cannot load this bitmap file. Use file of 16-bit color or 24-bit color mode with less or equal size 800x654.	6.6, chapter 8*
549	Cannot load this text file. Confirm the contents of file.	6.6, chapter 8*

* Features Guide, IM PX8000-01EN

Printer Errors

Code	Message	Chapter or Section
570	Close the printer cover.	21.1
571	Paper empty. Load a roll chart.	21.1
572	The printer head temperature is abnormality. Printing will be aborted. Printing will not be possible until the printer head temperature comes normal.	—
573	Printer over heat. Power off immediately.	—
574	Printer power supply error. Maintenance service is required.	—
575	Printer time out. Maintenance service is required.	—
576	Printer error.	—

Network Errors

Code	Message	Chapter or Section
600	Unable to connect to the server. Check the network settings and configuration.	Chapter 23
601	Has not connect with ftp server yet. Confirm the network settings and connection.	Chapter 23
602	This ftp function in not supported.	—
603	FTP Error: Client Handle Confirm the network settings and connection.	Chapter 23
604	Cannot send data to a network printer. Confirm the network settings and connection.	Chapter 23
608	Failed to acquire time from SNTP server. Confirm the network settings and connection.	Chapter 23

25.1 Messages and Corrective Actions

Execution Errors (650 to 799)

Code	Message	Chapter or Section
650	Data is invalid.	—
651	The option is not equipped, so it cannot execute.	—
652	Undo is not possible since data that existed immediately before initialization is not available.	—
653	Can not be executed while running. Press START/STOP key to stop acquisition.	4.2
654	Cannot manipulate files while image printing is in progress. Wait until image printing is complete.	—
656	Calibration failure. Disconnect the input and execute again. If it fails again, servicing is necessary.	24.1
660	Can not operate while data out. Wait until output is completed.	—
663	Cannot start.	—
664	GO/NO-GO is available while trigger mode is - 'Single' or 'Normal' - 'Auto' or 'AutoLevel' (Faster than 50ms/div)	3.1
666	Failed to measure statistics. Waveform data may be missing. If Cycle Statistics is specified, the instrument may be configured in a way that fails to detect the cycle.	14.2, 14.3
667	Executing file access. Abort or wait until it is complete.	—
668	Image is being printed or saved. Wait until the execution of the command is complete.	—
672	Cannot be executed when the time base setting is to be an External clock.	4.1
674	Average practice can't be done because the record length of the history exceeds the record length that it can be carried out.	20.1
675	Average practice can't be done because the record length of the history exceeds the record length that it can be carried out.	20.1
677	Cannot do while selftest is executing.	25.2
679	Cannot start at the current record length. Shorten the record length or meet the following condition. - Set the trigger mode to Auto, decrease T/Div to less than 100 msec/div to enable roll mode. - Set the trigger mode to Single or On Start.	2.8, 3.1
680	Averaging mode is not possible when the trigger mode is Single, SingleN, or On Start. Change the trigger mode.	3.1
684	Cannot start when the time base set to external clock while the acquisition mode set to envelope.	4.1
686	Cannot be executed when the acquisition mode is set to average. Change the mode.	4.1
693	Cannot be executed when GO/NO-GO mode is Zone.	17.1
695	Set acquisition mode to Normal when using a wave window trigger.	4.1
696	The wave window trigger cannot be used if the sampling rate is faster than 500 kS/s or slower than 10 kS/s.	2.8
702	All search conditions are OFF. At least one condition should ON.	Chapter 19, section 20.2
703	Display setting of search source is OFF. Set it to ON.	8.1
704	Cannot execute Time search while T/div is faster than 100msec/div.	2.8
705	Cannot start Action mode while trigger mode is SingleN.	3.1
706	Cannot be executed when GO/NO-GO mode is ON. Set the GO/NO-GO mode to OFF.	Chapter 17
707	Cannot execute search while searched No. reached Maximum(1000).	—
708	Cannot execute or set while AutoScroll processing. Stop AutoScroll.	12.1
712	Cannot start while No GO/NO-GO condition.	Chapter 17
713	Cannot make wave zone from less than 2,000 points data, from more than 10,000,000 points data, or from less than 10division data.	—
714	Cannot start Action mode while PrintImage target is "File". Change target to "printer".	21.2
716	Set the Math and FFT Window to OFF to Start GO/NO-GO.	Chapter 15, section 16.1
717	Cannot abort this process.	—

Code	Message	Chapter or Section
719	Cannot execute Time search when the time base setting is to be an External clock.	4.1
723	Cannot update null value. No measured value, calculated by numeric, is available to set.	24.2
724	Calibration error occurred. Restart this machine. If it occurred again, maintenance service is required.	—
725	Cannot execute when GO/NO-GO traces contain an AUX channel with the sense type set to pulse.	2.4 to 2.6
726	Cannot execute when search trace contains an AUX channel with the sense type set to pulse.	2.4 to 2.6
727	Cannot execute when trigger sources contain an AUX channel with the sense type set to pulse.	2.4 to 2.6
728	Cannot execute or change while running. Press the START/STOP key to stop acquisition.	4.2
729	No measurable channel.	—

Setup Errors (800 to 899)

Code	Message	Chapter or Section
800	Illegal date-time. Set the correct date and time.	—
801	Cannot set these file name. - Over 32 characters. - Include inhibit characters. - Inhibit MS-DOS file name. Enter an other file name.	22.3
803	Cannot change this parameter while running. Press the START/STOP key to stop acquisition.	4.2
804	Cannot change settings during GO/NO-GO. Stop the GO/NO-GO (Stop the Acquire).	Chapter 17
805	Can not change display points with this T/div setting.	2.8
806	Cannot be changed when trigger A is not X. Set the state of the channel corresponding to condition A to 'X'.	3.8 to 3.10
807	Cannot set while TimeSynchro setting not Off.	24.3
808	Cannot change when Channel Display is OFF or Math settings are invalid. Set the channel display ON or make appropriate Math settings.	8.1, chapter 15
809	Cannot change when External Clock is active.	4.1
810	Cannot change while running.	4.2
811	Illegal math expression. Input a correct computing equation.	15.5
812	Cannot set this model	—
813	Cannot set anything other than Low Pass for a Gaussian filter. Change the Filter Type to another filter besides Gaussian.	15.5
815	Cannot change settings during Action mode. Stop the Action.	18.1
816	Cannot set the channels which do not have modules installed.	Chapter 2, section 25.3
817	Cannot Set or Execute.	—
818	If the trigger mode is set to Single, Single(N), or OnStart, the acquisition mode cannot be set to Average.	3.1
819	If the acquisition mode is Average, the trigger mode cannot be set to Single, Single (N), or OnStart.	4.1
820	The acquisition mode cannot be set in the current record length.	4.1
822	Cannot be configured or executed during the search operation.	Chapter 19
823	Cannot be configured or executed during the history search operation.	20.2
824	The record cannot be selected.	Chapter 20
825	History record does not exist.	Chapter 20
826	Cannot be configured or executed while computation is in progress. Aborted when history display mode is set to One.	20.1
827	Cannot be configured or executed while updating the history all display. Aborted when history display mode is set to One.	20.1

25.1 Messages and Corrective Actions

Code	Message	Chapter or Section
829	Zones cannot be edited in the following cases: - When the main window is not displayed. - When the relevant waveform is not displayed.	5.1, 8.1, 11.1, 12.1, 16.1, 17.1
830	The zone waveform does not exist.	17.1
832	Zones determination is not possible in the following cases: - When the main window is not displayed. - When the relevant waveform is not displayed. - When the zone waveform does not exist.	5.1, 8.1, 11.1, 12.1, 16.1, 17.1
833	Processing statistics. To perform other operations, abort the statistical processing.	14.2
834	The channel which couldn't be set up was specified.	—
835	Cannot be set when the acquisition mode is set to average.	4.1
836	Cannot be changed when VScale is SPAN.	8.1
838	It is an unacceptable parameter to set up to the present module.	—*
840	Cannot be set to a range of 20 sec/div to 2 min/div during roll display.	2.8
842	Zooming is not available when the number of displayed points of the FFT waveform is less than 50 in the Zoom window.	12.1, 15.5, 16.1
846	P-P compression cannot be used to save when a record length is 1K.	—
852	Cannot set Math to OFF while FFT Window ON.	16.1
853	Cannot select this trace because it already selected.	—
855	Cannot change to such Record length while running. Set the trigger mode to Auto, decrease T/Div to less than 100 msec/div to enable roll mode, or set the trigger mode to Single or On Start.	2.8, 3.1
856	Cannot Display setting to ON. This CH didn't acquisition to memory.	—
858	Cannot set while action mode is ON.	18.1
867	Cannot be specified when the print style is Numeric.	—
869	Cannot set while GO/NO-GO mode. Turn OFF GO/NO-GO mode first.	Chapter 17
871	No effective channel for Math Setup.	—
872	No effective channel for History Search Setup.	—
874	Cannot set Save Range except 'Main' while PP-Comp save mode.	—
876	Cannot frame setting to ON, except Image format on JPEG.	21.3
877	Cannot set to display points under 100.	12.1
879	Cannot set GO/NO-GO mode while Math or FFT Window is ON.	Chapter 15, section 16.1
882	Cannot set while Single-N running.	3.1
890	Illegal math expression. Input a correct computing equation.	7.4
891	Cannot simultaneously set current range when sense types differ. To copy or set ranges to other current channels, first unify sense type.	2.2
892	Cannot set when current module types differ.	2.2
893	Cannot execute. Select copy destination channels(elements).	2.7

* Communication Interface User's Manual, IM PX8000-17EN

System Errors (900 to 999)

Code	Message	Chapter or Section
900	No module installed. Install the module.	2.3*
901	Failed to backup setup data. Will initialize. Backup battery may be low.	2.4*
902	The firmware is not suitable for this system. Install the proper firmware.	—
903	The USB device's power consumption exceeded the capacity of the USB hub.	7.9*
906	Fan stopped. Maintenance service is required.	—

* Getting Started Guide, IM PX8000-03EN

Code	Message	Chapter or Section
907	Internal temperature is too high. Maintenance service is required. It will shutdown automatically.	—
908	Check the measured current and the number of probes that you are using.	2.12*
910	Key protect is enabled. To release the protection, press the PROTECT key or enter the password.	24.9
911	Fan for Input modules stopped. Cannot start. Maintenance service is required.	—
912	Fan for CPU stopped. Maintenance service is required. It will shutdown automatically.	—
913	LCD BackLight Failure. Maintenance service is required.	—
914	Cannot start while this module configuration. 760811 should use in Slot 1,Slot 3,Slot 5,Slot 7. 760812 should use in Slot 2,Slot 4,Slot 6,Slot 8. 760813 should use in Slot 2,Slot 4,Slot 6,Slot 8. 760851 should use in Slot 3,Slot 5,Slot 7. Slot 1 and slot 2 must be installed.	2.3*
915	It installed the module which cannot support by this machine. Or it installed the module which cannot be used in the slot.	2.3*
917	Hardware configuration error occurred. Restart this machine. If it occurred again, maintenance service is required.	—
918	Error occurred while ImageFile process.	—
919	Key operate not available while system error occurred	—
920	Firmware overwriting error occurred.	—
922	Internal hardware communication error has occurred.	—
923	An error has occurred in the power measurement element. Power off immediately. Maintenance service is required.	—

* Getting Started Guide, IM PX8000-03EN

Note

If servicing is required, first see if initializing the instrument fixes the problem.

25.2 Carrying Out Self-Tests (Selftest)


This section explains the following settings for testing whether the PX8000’s keyboard, memory, SD card interface, and printer are functioning properly.

- Test type
- Executing tests

► [Features Guide: “Self-Test \(Self Test\)”](#)


UTILITY Self Test Menu

Press **UTILITY** and then the **Self Test** soft key to display the following menu.

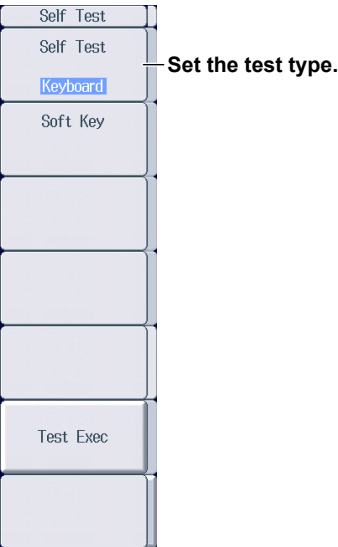


Setting the Test Type (Self Test)

Press the **Self Test** soft key to display the following menu.

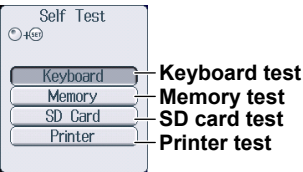


- Keyboard:** Tests whether or not the front panel keys are operating correctly and whether or not the soft keyboard accepts input properly. They are operating properly if the background color of the keys that you press changes from red to another color. The soft keyboard is operating properly if you can enter the specified characters.
- Memory:** Tests whether or not the internal CPU board RAM and ROM are operating properly. If they are operating properly, “Pass” appears. If an error occurs, “Error” appears.
- SD Card:** Tests whether the SD card interface is operating properly. If an error occurs, “Error” appears.
- Printer:** Tests whether or not the optional built-in printer is operating properly. The built-in printer is operating properly if the print density is correct. If an error occurs, the print density will not be correct.


Keyboard Test

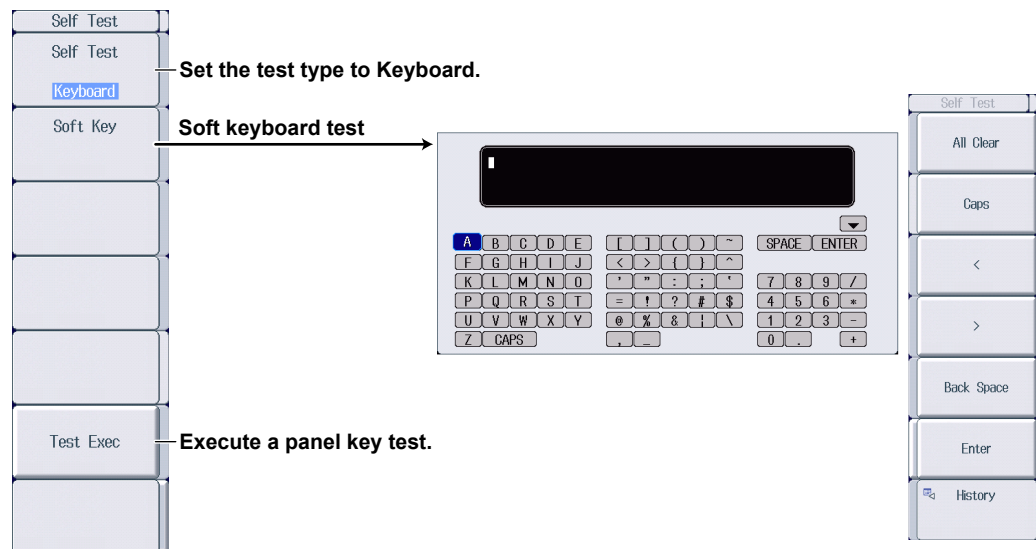


Memory Test

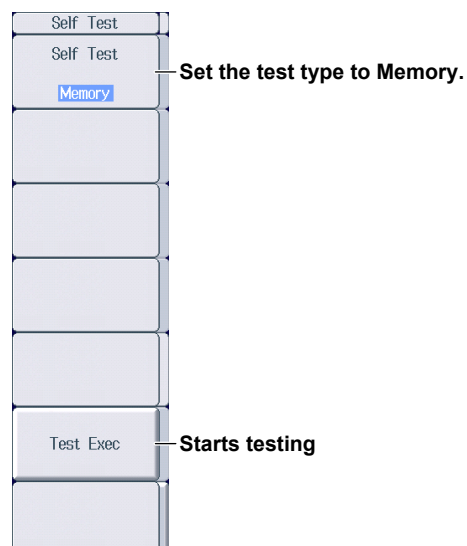

SD Card Test

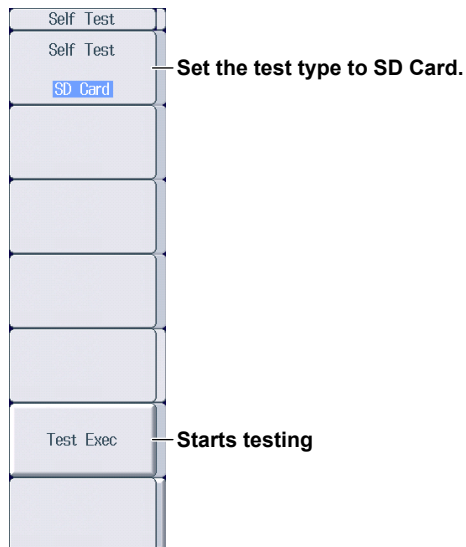

Printer Test

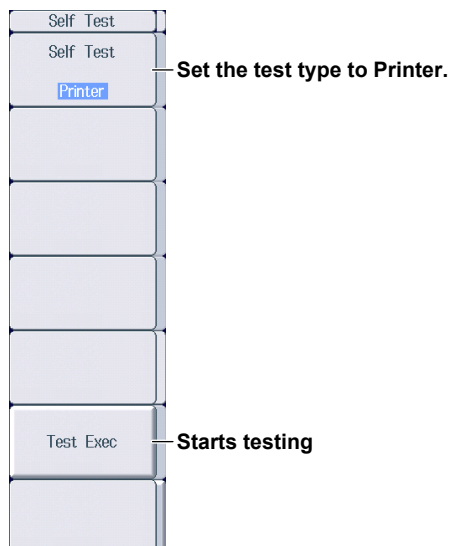

If an Error Occurs during a Self-Test

If an error occurs even after you carry out the following procedure, contact your nearest YOKOGAWA dealer.

- Execute the self-test again several times.
- Confirm whether or not the media being tested is properly inserted.
- Check that the paper is set properly in the built-in printer and that paper is not jammed.

25.3 Viewing System Information (Overview)

This section explains how to view the PX8000 system information.

► Features Guide: “Overview (Overview)”

Viewing System Information (Overview)

Press **UTILITY** and then the **Overview** soft key to display the following screen.

Overview				
-Model		PX8000	RecordLength 100Mpts/CH	
Serial No / ProductID		91NA16947 / 7WGBCS2Z (MAC:00016494004)		
-Slot	Model	Serial No	/Pair Serial No	Adjustment Date
1:	760811	91NA16919/91NA16867		2013/12/25 19:28:34
2:	760812	91NA16867/91NA16919		2013/12/25 19:28:34
3:	760811	91NA16921/91NA16869		2013/12/25 19:28:36
4:	760812	91NA16869/91NA16921		2013/12/25 19:28:36
5:	760811	91NA16922/91NA16870		2013/12/25 19:28:40
6:	760812	91NA16870/91NA16922		2013/12/25 19:28:40
7:	760851			
8:	-			
-Options				
/M2	Memory expansion 100Mpts/CH			
/B5	Built-in printer			
/C20	IRIG interface			
/G5	Harmonic Measurement			
/P4	4 Probe power outputs			
-Default Language English				
-Information				
Firm Version	2.01	14/08/01 12:00		
FPGA1 Version	ACQC(1.00.01, 20131209)	PCI(1.00.01, 20131212)		
FPGA2 Version	WATT[190](0.00.20)	GDC(0.50)	CIO(0.38)	

Displayed Information

Model, Record Length	Model and record length
Serial No / ProductID	Serial number and product number
Slot	Model and serial number of the module installed in each slot
Options	Installed options
Default Language	Default language
Information	Firmware and FPGA versions and other information

Index

Numerics Page

4-, 8-, and 16-value displays 6-3

A Page

ACQUIRE menu 4-1
 acquisition mode 4-2
 action 18-2
 action conditions 17-3
 action execution save destination 22-10
 ACTION menu 18-1
 action, setting (Action Setup) 18-1
 action to perform at power on 24-7
 All Items display 6-7
 ALL SET and ALL RESET 22-28
 apparent power equation 7-6
 applicable standard (corrected power) 7-6
 arrow keys v
 Auto Level (trigger mode) 3-1
 automated measurement of waveform parameters, saving
 results of 22-15
 auto naming 22-8
 auto scroll 12-3
 Auto (trigger mode) 3-1
 Average (acquisition mode) 4-2

B Page

background 6-10
 B Between (determination mode) 3-16
 B < Time (determination mode) 3-16
 B > Time (determination mode) 3-16
 B TimeOut (determination mode) 3-16

C Page

cable 23-1
 calibration 24-1
 CAL menu 24-1
 character strings, entering viii
 clear trace 8-3
 click sound 24-8
 color 22-16
 color (waveform) 8-1
 column (Matrix display) 6-5
 combine display 11-1
 comment 22-8
 computation 15-1, 15-2, 15-3, 15-4, 15-6
 connection, items required 23-1
 connection procedure 23-2
 constant 15-7
 CURSOR Degree menu 13-5
 CURSOR Horizontal menu 13-1
 CURSOR H & V menu 13-6
 CURSOR Marker menu 13-3
 CURSOR Peak menu 13-7
 CURSOR Vertical menu 13-2
 Custom display 6-10
 customization 6-10
 cycle trace 14-5

D Page

data format (Format) 22-16
 data type (Data Type) 22-6

data type to save 22-16
 date and time 3-5
 delay 14-3
 determination mode (period trigger) 3-14
 determination mode (pulse width trigger) 3-16
 display, changing (4-, 8-, and 16-value displays) 6-3
 display, changing (All Items display) 6-7
 display, changing (Matrix display) 6-5
 display configuration 6-10
 displayed digits 24-8
 displayed harmonics 9-1
 displayed page, switching 6-1
 display format (bar graph) 9-1
 display format (file list) 22-23
 display format (phase difference) 7-8
 display format (vectors) 10-1
 display format (waveform) 8-1
 display (harmonics list) 6-8
 display mode (history waveform) 20-1
 DISPLAY MODE menu 5-1
 display position 6-10
 DISPLAY SETTING menu 5-1
 distortion factor equation 7-9
 DNS 23-3

E Page

element information 24-2
 ENHANCED_A->B(N) Trigger menu 3-8
 ENHANCED A Delay B Trigger menu 3-9
 ENHANCED AND Trigger menu 3-12
 ENHANCED Edge On A Trigger menu 3-10
 ENHANCED OR Trigger menu 3-11
 ENHANCED Period Trigger menu 3-13
 ENHANCED Pulse Width Trigger menu 3-15
 ENHANCED Wave Window Trigger menu 3-17
 Envelope (acquisition mode) 4-2
 equation 7-4, 7-6
 Error Messages 25-1
 ESC key v
 Ethernet interface specifications 23-1
 execution errors 25-4
 expression 15-6
 external I/O terminal 24-8
 extra window 8-1

F Page

FFT analysis results, saving 22-15
 FFT conditions 16-2
 FFT menu 16-1
 FFT (user-defined computation) 15-7
 file and folders, deleting 22-25
 file errors 25-2
 file list 22-22
 file list, sorting 22-23
 file names 22-7
 FILE Numeric Save menu 22-11
 FILE Others Load menu 22-21
 FILE Others Save menu 22-15
 files and folders, renaming 22-25
 files, copying 22-26
 file, selecting 22-19, 22-20, 22-21
 FILE Setup Load menu 22-20
 FILE Setup Save menu 22-14

Index

files, moving.....	22-27
FILE Utility menu	22-28
FILE Waveform Load menu	22-19
FILE Waveform Save menu	22-6
filter	15-7
folders (directories), creating	22-26
font color	6-10
font size	6-10, 24-8
FTP client software	23-4
FTP server	23-4

G Page

GO/NO-GO menu (waveform parameter)	17-4
GO/NO-GO menu (waveform zone)	17-1
grid	8-1

H Page

harmonic measurement	7-9
harmonics list	6-8
history data range (save)	22-9
HISTORY menu	20-1, 20-3
history waveform list (List)	20-2
hold-off time	3-3

I Page

information	25-1
initialization	24-6
intensity	24-8
interpolation method (waveform)	8-1
interpolation method (X-Y)	11-1
IRIG	24-3

J Page

jog shuttle	vii
judgment conditions	17-2, 17-5

K Page

keyboard	viii
keyboard test	25-9
key lock	24-10
key lock type	24-8
key operations	iv
keypad	vii

L Page

language	24-4
list number	6-8
loading (setup file)	22-20
loading (snapshot waveform file)	22-21
loading (waveform file)	22-19

M Page

magnification	12-4
mapping (waveform)	8-1
MATH menu (addition, subtraction, multiplication, division) ..	15-1
MATH menu (binary conversion)	15-2
MATH menu (phase shift)	15-3
MATH menu (power spectrum)	15-4
MATH menu (user-defined computation)	15-5
Matrix display	6-5
measure data, saving	22-6
measured harmonic order	7-9
measured results	14-6
measurement items	14-2
MEASURE menu (automated measurement)	14-1

MEASURE menu (cycle statistics)	14-5
MEASURE menu (normal statistics)	14-4
medium (drive), changing	22-24
memory test	25-9
menu background color	24-8
messages	25-1
MODE menu	3-1

N Page

network drive	23-5
network errors	25-3
Normal (acquisition mode)	4-2
Normal (trigger mode)	3-1
NULL feature	24-2
number of digits to display for numeric data	24-8
numeric data, saving	22-11
numeric display frame	24-8
NUMERIC key	7-1

O Page

On Start (trigger mode)	3-1
-------------------------------	-----

P Page

page, switching	6-1
phase difference	7-8
PLL source	7-9
POSITION/DELAY menu	3-2
print	21-3
printer errors	25-3
printer roll paper	21-1
printer test	25-10
PRINT MENU menu (built-in printer)	21-3
PRINT MENU menu (file saving)	21-4
protection, turning on and off	22-28

R Page

release type (key lock)	24-8
reset (4-, 8-, and 16-value displays)	6-3
RESET key	v
reset (Matrix display)	6-5
response time (start/stop)	24-8
roll paper handling	21-1
roll paper, loading	21-2

S Page

save (FILE menu, numeric)	22-11
save (FILE menu, others)	22-15
save (FILE menu, setup)	22-14
save (FILE menu, waveform)	22-6
SAVE menu (Image)	21-5
SAVE menu (Numeric)	22-12
SAVE menu (Waveform)	22-10
save (PRINT key)	21-4
save (SAVE key, Image Save)	21-5
save (SAVE key, numeric)	22-12
save (SAVE key, waveform)	22-10
scale value	8-1
scale value display	24-8
screen capture save destination and file name	21-5
screen capture, saving	22-15
SD card test	25-10
SD memory card	22-1
search conditions (edge)	19-1
search conditions (history waveform)	20-4
search conditions (time)	19-3
search (edge)	19-2

SEARCH Edge menu	19-1
search (history waveform)	20-5
search (time)	19-3
SEARCH Time menu	19-3
search zero cross	7-2
self-test, if an error occurs	25-10
sequence	17-3
SET key	v
SET/RESET	22-28
settings, initialization	24-6
setup data loading	22-20
setup data, saving	22-14
setup errors	25-5
SIMPLE/ENHANCED menu	3-3
SIMPLE External menu	3-6
SIMPLE Line Menu	3-7
SIMPLE menu (edge trigger)	3-4
SIMPLE Time menu	3-5
SingleN (trigger mode)	3-1
Single (trigger mode)	3-1
snapshot	8-3
snapshot waveforms, loading	22-21
snapshot waveforms, saving	22-15
SNTP	23-6
source waveform and measurement items	14-2
source waveform and parameter (history waveform)	20-4
source waveform (angle cursor)	13-5
source waveform (horizontal and vertical cursors)	13-6
source waveform (horizontal cursor)	13-1
source waveform (marker cursor)	13-4
source waveform (vertical cursor)	13-2
specified channels, copying to	14-3
standard (corrected power)	7-6
start and stop response time	24-8
state condition (A -> B trigger)	3-8
state condition (A Delay B trigger)	3-9
state condition (AND trigger)	3-12
state condition (Edge On A trigger)	3-10
state condition (OR trigger)	3-11
state condition (period trigger)	3-13
state condition (pulse width trigger)	3-15
storage management	22-5
storage medium to format	22-5
system errors	25-6
system information	25-11

T	Page
T1 < T < T2 (determination mode)	3-14
TCP/IP	23-3
terminal	24-8
test type (self-test)	25-8
TIME/DIV display	2-31
time scale	2-31
trace label	8-1
trigger condition (A -> B trigger)	3-8
trigger condition (A Delay B trigger)	3-9
trigger condition (AND trigger)	3-12
trigger condition (Edge On A trigger)	3-10
trigger condition (OR trigger)	3-11
trigger condition (period trigger)	3-13
trigger condition (pulse width trigger)	3-15
trigger condition (wave window trigger)	3-17
trigger mode	3-1
T < T1, T2 < T (determination mode)	3-14
T < Time (determination mode)	3-14
T > Time (determination mode)	3-14

type of file to list, selecting	22-24
---------------------------------------	-------

U	Page
USB keyboard	24-4
USB storage device	22-3
user-defined function	7-4
UTILITY Network Menu (FTP Server)	23-4
UTILITY Network menu (net drive)	23-5
UTILITY Network menu (SNTP)	23-6
UTILITY Network Menu (TCP/IP)	23-3
UTILITY Preference menu	24-7
UTILITY Self Test menu	25-8
UTILITY Store/Recall menu	24-9
UTILITY System Config All Setup menu	24-6
UTILITY System Config LCD menu (backlight)	24-5
UTILITY System Config menu (format)	22-4
UTILITY System Config menu (language)	24-4
UTILITY System Config Time Synchro menu	24-3

V	Page
vertical position (current)	2-7
vertical position (power)	2-9
vertical position (rotating speed)	2-21
vertical position (sensor input voltage)	2-15
vertical position (torque)	2-27
vertical position (voltage)	2-3

W	Page
waveform acquisition	4-3
waveform data loading	22-19
waveform parameters	17-5
waveform parameter search (history waveform)	20-4
waveform save conditions	22-8
waveform save range	22-7
waveforms, clearing	22-19, 22-21
waveforms to save	22-9
waveform vertical position (current)	2-7
waveform vertical position (power)	2-9
waveform vertical position (rotating speed)	2-21
waveform vertical position (sensor input voltage)	2-15
waveform vertical position (torque)	2-27
waveform vertical position (voltage)	2-3
waveform zone, editing	17-2
window layout (X-Y)	11-1

X	Page
X-Y menu	11-1
X-Y window	11-1

Z	Page
zone, editing	17-2
zone search (history waveform)	20-4
ZOOM menu	12-1
zoom position	12-4
zoom source waveforms	12-3